

# **Data Report**

## **NBP0305A**

**Dec 18, 2003 – Jan 2, 2004**



Photo by Sarah Riseman

**United States Antarctic Program**

**RVIB Nathaniel B. Palmer**

**Raytheon Polar Services**

Data Report Prepared by:  
Kathleen Gavahan and Dean Klein



## Table of Contents

<b>INTRODUCTION.....</b>	<b>1</b>
<b>DISTRIBUTION CONTENTS AT A GLANCE .....</b>	<b>2</b>
EXTRACTING DATA.....	2
<b>DISTRIBUTION CONTENTS .....</b>	<b>3</b>
CRUISE INFORMATION.....	3
<i>Cruise Track</i> .....	3
<i>Satellite Images</i> .....	3
NBP DATA PRODUCTS .....	3
<i>JGOFS</i> .....	3
<i>MGD77</i> .....	4
SCIENCE OF OPPORTUNITY .....	5
<i>ADCP</i> .....	5
<i>PCO<sub>2</sub></i> .....	5
CRUISE SCIENCE .....	6
<i>CTD</i> .....	6
<i>XBT</i> .....	6
RVDAS .....	6
<i>Sensors and Instruments</i> .....	6
Underway Sensors .....	6
Meteorology and Radiometry.....	6
Geophysics .....	7
Oceanography.....	7
Navigational Instruments .....	7
<i>Data</i> .....	7
Underway Data .....	8
Meteorology (met1).....	8
Gravimeter (grv1).....	8
Bathy 2000 (bat1).....	9
Simrad (sim1).....	10
Thermosalinograph (tsg1) .....	10
Fluorometer (flr1).....	10
pCO <sub>2</sub> .....	11
Navigational Data .....	11
Seapath GPS (seap) .....	11
Ashtech GPS (3df1).....	13
Trimble GPS (PCOD) .....	14
Gyro Compass (gyr1) .....	16
ADCP Course (adcp).....	16
Sound Velocity Probe (svp1).....	16
PROCESS .....	16
pCO <sub>2</sub> -merged .....	16
tsgfl.....	17
<b>CALCULATIONS.....</b>	<b>18</b>
TSG .....	18
PAR .....	18
PIR.....	19
PSP .....	19
<b>ACQUISITION PROBLEMS AND EVENTS.....</b>	<b>20</b>
<b>APPENDIX: SENSORS AND CALIBRATIONS.....</b>	<b>21</b>
NBP0305A SENSORS: .....	21
<i>Shipboard Sensors</i> .....	21
<i>CTD</i> .....	22

CALIBRATIONS .....	23
CTD .....	23
<i>Pressure Sensor</i> .....	23
<i>Primary Temperature Sensor</i> .....	24
<i>Secondary Temperature Sensor</i> .....	24
<i>Dissolved Oxygen Sensor</i> .....	25
<i>Fluorometer</i> .....	27
<i>Transmissometer</i> .....	29
<i>Primary Conductivity Sensor</i> .....	30
<i>Secondary Conductivity Sensor</i> .....	31
METEOROLOGY SYSTEM .....	32
<i>Anemometer (Port)</i> .....	32
<i>Anemometer (Starboard)</i> .....	33
<i>PIR</i> .....	34
<i>PSP</i> .....	35
<i>PAR</i> .....	36
TSG CALIBRATION FILES .....	38
<i>Underway Conductivity Sensor</i> .....	38
<i>Underway Temperature Sensor</i> .....	40
<i>Underway Remote Temperature Sensor</i> .....	42
<i>Underway Transmissometer</i> .....	43
<i>Gravity Tie Meter</i> .....	44

## Introduction

The NBP data acquisition systems continuously log data from the instruments used during the cruise. This document describes:

- The structure and organization of the data on the distribution media
- The format and contents of the data strings
- Formulas for calculating values
- Information about the specific instruments in use during the cruise
- A log of acquisition problems and events during the cruise that may affect the data
- Scanned calibration sheets for the instruments in use during the cruise.

The data is distributed on a CD-R written in ISO9660 level-1 format. It is readable by virtually every computing platform.

All the data has been compressed using Unix "gzip," identifiable by the ".gz" extension. It has been copied to the distribution media in the Unix tar archive format, ".tar" extension. Tools are available on all platforms for uncompressing and de-archiving these formats: On Macintosh, use Stuffit Expander with DropStuff. On Windows operating systems use WinZip.

*IMPORTANT: Read the last section, "Acquisition Problems and Events," for important information that may affect the processing of this data.*

## Distribution Contents at a Glance

### Volume 1

```
process/ 305Ajgof.tar
         305Amgd.tar
         305Aproc.tar
         305Apco2.tar
         305Aqcps.tar

NBP305A.trk
NBP305A.mgd
NBP305A.gmt

plots/   Cruise Plots

rvdas/uw/ 305Abat.tar
         305Aflr.tar
         305Amet.tar
         305Apco2.tar
         305Asim.tar
         305Asvp.tar
         305Atsg.tar
         305Agrv.tar
         305Ambdp.tar
```

### Volume 2

```
rvdas/nav/305Aadu.tar
         305Aadcp.tar
         305Agyr.tar
         305Aseap.tar
         305APCOD.tar

adcp/    pingdata files
         config files

imagery/ TeraScan satellite images

ocean/   305Actd.tar
         305Axbt.tar

report/   NBP0305A.doc
         rvdascal.txt

science/ science.tar
```

## Extracting Data

The Unix tar command has many options. It is often useful to know exactly how an archive was produced when expanding its contents. All archives were created using the command,

```
tar cvf archive_filename files_to_archive
```

To create a list of the files in the archive, use the Unix command,

```
tar tvf archive_filename > contents.list
```

where `contents.list` is the name of the file to create

To extract the files from the archive:

```
tar xvf archive_filename file(s)_to_extract
```

G-zipped files will have a “.gz” extension on the filename. These files can be decompressed after de-archiving, using the Unix command,

```
gunzip filename.gz
```

## Distribution Contents

### Cruise Information

#### *Cruise Track*

The distribution CD includes a GMT cruise track file (NBP0305A.trk). It contains the longitude and latitude at one-minute intervals extracted from the NBP0305A.gmt file.

One PostScript cruise track file has been produced and placed in the /plots directory. The plot is standard US Letter sized (8.5" x 11").

#### *Satellite Images*

Satellite Images processed for this cruise can be found in the directory imagery tar files, ice and wx (weather). Files are named using the convention, IdDDYYA.jpg where:

Id = image type (is = ice ssmi, iv = ice visible, cw = seawifs, wx = weather)

DDD = year-day

YY = year

A = allows for multiple images of one type for one day

### NBP Data Products

Two datasets are created on each cruise: JGOFS and MGD77.

#### *JGOFS*

The JGOFS data set can be found on the distribution media in the file /process/<cruisen>.tar. The archive contains a single file produced each day named jgDDD.dat.gz where DDD is the year-day the data was acquired. The ".gz" extension indicates that the individual files are compressed before archiving. The daily file consists of 22 columnar fields in text format described in the table below. The JGOFS data set is obtained primarily by applying calibrations to raw data and decimating to whole minute intervals. Several fields are derived measurements from more than a single raw input. For example, Course Made Good (CMG) and Speed Over Ground (SOG) are calculated from gyro and GPS inputs. During the cruise, the JGOFS data set produces the daily data plots. Note: Null, unused, or unknown fields are indicated as "NAN" in the JGOFS data.

Field	Data	Units
01	GMT date	dd/mm/yy
02	GMT time	hh:mm:ss
03	NGL latitude (negative is South)	tt.tttt
04	NGL longitude (negative is West)	ggg.gggg
05	Speed over ground	Knots
06	GPS HDOP	-
07	Gyro Heading	Degrees (azimuth)
08	Course made good	Degrees (azimuth)
09	Mast PAR	$\mu$ Einsteins/meter <sup>2</sup> sec
10	Sea surface temperature	°C
11	Sea surface conductivity	siemens/meter
12	Sea surface salinity	PSU
13	Sea depth (uncorrected, calc. sw sound vel. 1500 m/s)	meters
14	True wind speed (port windbird)	meters/sec

Field	Data	Units
15	True wind direction (port windbird)	degrees (azimuth)
16	Ambient air temperature	°C
17	Relative humidity	%
18	Barometric pressure	MBar
19	Sea surface fluorometry	volts (0-5 FSO)
20	Not used	-
21	PSP	W/m <sup>2</sup>
22	PIR	W/m <sup>2</sup>

## MGD77

The MGD77 data set is contained in a single file for the entire cruise. It can be found in the top level of the distribution data structure as NBP305A.mgd. Also at the root level, NBP305A.gmt is the output of the mgd77togmt utility using NBP305A.mgd as input. The NBP305A.gmt file can be used with GMT plotting software.

The data used to produce the NBP305A.mgd file can be found on the distribution media in the file /process/305Aproc.tar. The data files in the archive contain a day's data and follow the naming convention Dddd.fnl.gz, where ddd is the year-day. These files follow a space-delimited columnar format that may be more accessible for some purposes. They contain data at one-second intervals rather than one minute and are individually "gzipped" to save space. Below is a detailed description of the MGD77 data set format. The other files in the archive contain interim processing files and are included to simplify possible reprocessing of the data using the RVDAS NBP processing scripts.

All decimal points are implied. Leading zeros and blanks are equivalent. Unknown or unused fields are filled with 9's. All "corrections", such as time zone, diurnal magnetics, and EOTVOS, are understood to be added.

Col	Len	Type	Contents	Description, Possible Values, Notes
1	1	Int	Data record type	Set to "5" for data record
2-9	8	Char	Survey identifier	
10-12	3	int	Time zone correction	Corrects time (in characters 13-27) to GMT when added; 0 = GMT
13-16	4	int	Year	4 digit year
17-18	2	int	Month	2 digit month
19-20	2	int	Day	2 digit day
21-22	2	int	Hour	2 digit hour
23-27	5	real	Minutes x 1000	
28-35	8	real	Latitude x 100000	+ = North - = South. (-9000000 to 9000000)
36-44	9	real	Longitude x 100000	+ = East - = West. (-18000000 to 18000000)
45	1	int	Position type code	1=Observed fix 3=Interpolated 9=Unspecified
46-51	6	real	Bathymetry, 2- way travel time	In 10,000th of seconds. Corrected for transducer depth and other such corrections
52-57	6	real	Bathymetry, corrected depth	In tenths of meters.
58-59	2	int	Bathymetric correction code	This code details the procedure used for determining the sound velocity correction to depth
60	1	int	Bathymetric type code	1 = Observed 3 = Interpolated (Header Seq. 12) 9 = Unspecified
61-66	6	real	Magnetics total field,	In tenths of nanoteslas (gammas)

Col	Len	Type	Contents	Description, Possible Values, Notes
			1 <sup>st</sup> sensor	
67-72	6	real	Magnetics total field, 2 <sup>nd</sup> sensor	In tenths of nanoteslas (gammas), for trailing sensor
73-78	6	real	Magnetics residual field	In tenths of nanoteslas (gammas). The reference field used is in Header Seq. 13
79	1	int	Sensor for residual field	1 = 1 <sup>st</sup> or leading sensor 2 = 2 <sup>nd</sup> or trailing sensor 9 = Unspecified
80-84	5	real	Magnetics diurnal correction	In tenths of nanoteslas (gammas). (In nanoteslas) if 9-filled (i.e., set to "+9999"), total and residual fields are assumed to be uncorrected; if used, total and residuals are assumed to have been already corrected.
85-90	6	F6.0	Depth or altitude of magnetics sensor	(In meters) + = Below sea level 3 = Above sea level
91-97	7	real	Observed gravity	In 10 <sup>th</sup> of mgals. Corrected for Eotvos, drift, tares
98-103	6	real	EOTVOS correction	In 10 <sup>th</sup> of mgals. $E = 7.5 V \cos \phi \sin \alpha + 0.0042 V^*V$
104-108	5	real	Free-air anomaly	In 10 <sup>th</sup> of mgals G = observed G = theoretical
109-113	5	char	Seismic line number	Cross-reference for seismic data
114-119	6	char	Seismic shot-point number	
120	1	int	Quality code for navigation	5= Suspected, by the originating institution 6= Suspected, by the data center 9= No identifiable problem found

## Science of Opportunity

### ADCP

The shipboard ADCP system measures currents in the depth range from about 30 to 300 m -- in good weather. In bad weather or in ice, the range is less, and sometimes no valid measurements are made. It is the USAP-funded project of Eric Firing (University of Hawaii) and Teri Chereskin (Scripps Institution of Oceanography). ADCP data collection occurs on the both LMG and the NBP for the benefit of the scientists on individual cruises, and for the long-term goal of building a climatology of current structure in the Southern Ocean.

The ADCP data set collected during this cruise has been placed on the distribution media in the archive /adcp/305Aadcp.tar. The archive consists of a single file for each day of data collection. The files are named PINGDATA.xxx where xxx is a day number that is NOT a year-day. For the date, use the file's creation date.

Some ADCP data is also transmitted to RVDAS. East and north vectors for ship's speed relative to the reference layer and ship's heading are archived as 305Aadcp.tar in the directory /rvdas/nav.

### PCO<sub>2</sub>

The NBP carries Lamont-Doherty Earth Observatory's (LDEO) pCO<sub>2</sub> system and RPSC staff maintains it. Data is sent to LDEO at the end of each cruise. The pCO<sub>2</sub> data is transmitted and archived on RVDAS. You will find it in a file named 305Apco2.tar in

the `process/` directory, which contains the pCO<sub>2</sub> instrument's data merged with GPS, meteorological and other oceanographic measurements. For more information contact Colm Sweeney (csweeney@ldeo.columbia.edu) for additional information.

## Cruise Science

### CTD

The CTD data have been placed in the tar file `/ocean/305Actd.tar`.

### XBT

The XBT data have been placed in the tar file `/ocean/305Axbt.tar`.

### RVDAS

The Research Vessel Data Acquisition System (RVDAS) was developed at Lamont-Doherty Earth Observatory of Columbia University and has been in use on its research ship for many years. It has been modified for use on the USAP research vessels.

Daily data processing of the RVDAS (Research Vessel Data Acquisition System) data is performed to convert values into useable units and as a check of the proper operation of the DAS. Both raw and processed data sets from RVDAS are included in the data distribution. The tables below provide detailed information on the data. Be sure to read the "Significant Acquisition Events" section for important information about data acquisition during this cruise.

### Sensors and Instruments

RVDAS data is divided into two general categories, *underway and navigation*. They can be found on the distribution media as subdirectories under the top level `rvdas` directory: `/rvdas/uw`, and `/rvdas/nav`. Processed oceanographic data is in the top level directory, `/process`. Each instrument or sensor produces a data file named with its channel ID. Each data file is g-zipped to save space on the distribution media. Not all data types are collected every day or on every cruise.

The naming convention for data files produced by the sensors and instruments is

NBP[CruiseID][ChannelID].dDDD

Example: NBP0107.met1.d317

- The CruiseID is the numeric name of the cruise, in this case, NBP0305A.
- The ChannelID is a 4-character code representing the system being logged. An example is "met1," the designation for meteorology.
- DDD is the day of year the data was collected

## Underway Sensors

### Meteorology and Radiometry

Measurement	Channel ID	Collect. Status	Rate	Instrument
Air Temperature	met1	continuous	1 sec	R. M. Young 41372LC
Relative Humidity	met1	continuous	1 sec	

Measurement	Channel ID	Collect. Status	Rate	Instrument
Wind Speed/Direction	met1	continuous	1 sec	R.M. Young 05106
Barometer	met1	continuous	1 sec	R.M. Young 61201
PIR (LW radiation)	met1	continuous	1 sec	Eppler PIR
PSP (SW radiation)	met1	continuous	1 sec	Eppler PSP
PAR	met1	continuous	1 sec	BSI QSR-240
GUV	guv	not collected	2 sec	BSI PUV-511
PUV	puv	not collected	On casts	BSI PUV-500

## Geophysics

Measurement	Channel ID	Collect. Status	Rate	Instrument
Gravimeter	grv1	collected	10 sec*	LaCoste & Romberg
Magnetometer	mag1	not collected	15 sec	EG&G G-866
Bathymetry	bat1	continuous	Varies	ODEC Bathy 2000
Bathymetry	knu1	not collected	Varies	Knudsen 320B/R
Bathymetry	sim1	collected occasionally	Varies	Simrad EK500 Sonar

\*Data is output every second but it only changes every 10 seconds.

## Oceanography

Measurement	Channel ID	Collect. Status	Rate	Instrument
Conductivity	tsg1	Continuous	6 sec	SeaBird 21
Salinity	tsgfl	Continuous	6 sec	Calc. from pri. temp
Sea Surface Temp	tsg1	Continuous	6 sec	SeaBird 3-01/S
Fluorometry	flr1	Continuous	1 sec	Turner 10-AU-005
Fluorometry	flr1 & tsg1	Continuous	6 sec	
Transmissometry	tsg1	Continuous	6 sec	WET Lab C-Star
pCO <sub>2</sub>	pco2	Continuous	70 sec	(LDEO)
ADCP	adcp	Continuous	varies	RD Instruments

## Navigational Instruments

Measurement	Channel ID	Collect. Status	Rate	Instrument
Attitude GPS	Adu1	continuous	1 sec	Ashtech ADU2
Trimble GPS	PCOD	Continuous	1 sec	Trimble 20636-00SM
Gyro	gyr1	Continuous	0.2 sec	Yokogawa Gyro
SeaPath	Seap	Continuous	1 sec	SeaPath 200

## Data

Data is received from the RVDAS system via RS-232 serial connections. A time tag is added at the beginning of each line of data in the form,

```
yy+dd:hh:mm:ss.sss [data stream from instrument]
```

where

yy = two-digit year

ddd = day of year

hh = 2 digit hour of the day

mm = 2 digit minute

ss.sss = seconds

All times are reported in UTC.

The delimiters that separate fields in the raw data files are often spaces and commas but can be other characters such as : = @. Occasionally no delimiter is present. Care should be taken when reprocessing the data that the field's separations are clearly understood.

In the sections below a sample data string is shown, followed by a table that lists the data contained in the string.

## Underway Data

### Meteorology (met1)

01+322:00:03:27.306 04.5 292 010 05.7 294 010 0959.6 000.2 093 -000.1537  
0001.0886 0012.8248

Field	Data	Units
1	RVDAS time tag	
2	Port anemometer speed (relative)	m/s
3	Port anemometer direction (relative)	deg
4	Port anemometer standard deviation	deg
5	Starboard anemometer speed (relative)	m/s
6	Starboard anemometer direction (relative)	deg
7	Starboard anemometer standard deviation	deg
8	Barometer	mBar
9	Air temperature	°C
10	Relative humidity	%
11	PSP (short wave radiation)*	mV
12	PIR (long wave radiation)*	mV
13	PAR (photosynthetically available radiation)*	mV

\*See page 18 for calculations.

### Gravimeter (grv1)

99+099:00:18:19.775 your\_line#1999 99 01818 9735.4

Field	Data	Conversion	Units
1	RVDAS time tag		
2	Text string		
3	Gravity device date	yyyymmddhhmmss	
4	Gravity count	mgal = count x 1.0047 + offset	count

**Bathy 2000 (bat1)**

00+019:23:59:53.901 ;I04485.3ME -23.0, I00000.0,-99.9,0000@01/11/00,  
 23:59:52.08 PW2 PF1 SF1 PL3 MO4 SB3 PO0 TX1 TR: GM5 1500 06.7 -72.1

Field	Data	Format / Possible Values	Units
1	RVDAS time tag		
2	Flagged low frequency chn. depth w/ units	;FDDDDD.Dun where F = flag (V for valid, I for invalid), D=depth, un = units	meters
3	Low Frequency echo strength	EEE.EE	dB
4	Flagged high freq. chn. depth	not used	
5	High frequency echo strength	not used	
6	Signed heave data	SHHHH	cm
7	Date	mm/dd/yy	
8	Time	hh:mm:ss	
9	Transmit pulse window type	PW1=Rectangular PW2=Hamming PW3=Cosine PW4=Blackman	
10	Primary transmit frequency	PF1=3.5 kHz PF2=12.0 kHz	kHz
11	Parametric mode secondary frequency	SF1=3.5 kHz SF2=12.0 kHz	kHz
12	Pulse length	PL1=200usec PL2=500usec PL3=1msec PL4=2msec PL5=5msec PL6=10msec PL7=25msec If transmit mode is FM: PL1=25msec PL2=50msec PL3=100msec	
13	Operating mode	MO1=CW parametric MO2=CW MO3=FM parametric MO4=FM	
14	Frequency sweep bandwidth	SB1=1 kHz SB2=2 kHz SB3=5 kHz	kHz
15	Power level	PO1 = 0dB PO2 = -6dB PO3 = -12dB PO4 = -18dB PO5 = -24dB PO6 = -30dB PO6 = -30 dB PO7 = -36dB PO8 = -42dB	
16	Transmit mode	TX1=single ping active TX2=pinger listen TX3=multipinging TR TX4=multipinging TR TX5=multipinging TTRR TX6=multipinging TTTTRRRR	

Field	Data	Format / Possible Values	Units
17	Transmit Rate	TX7=multipinging TTTTTRRRRR TR3 = 4Hz TR4 = 2Hz TR5 = 1Hz TR6 = .5Hz TR7 = .33Hz TR8 = .25Hz TR9 = .20Hz TR: = .10Hz TR; = .05Hz	Hz
18	System gain mode	GM0=hydrographic AGC GM1 to GM9=hydrographic +3db to + 27db manual. GMA to GMD=hydrographic + 30db through + 60db manual GME to GMK=sub-bottom 1 through sub-bottom 7	
19	Speed of sound		m/sec
20	Depth of sonar window below sea-level		meters
21	Background noise level in fixed point reference		dB/V

### Simrad (sim1)

00+005:00:00:52.388 D1,23583509,1479.6, 17, 1, 0

Field	Data	Units
1	RVDAS time tag	
2	Header	
3	Time tag	hhmmss.sss
4	Depth	m
5	Bottom surface backscattering strength	dBar
6	Transducer number ( 1 = 38 kHz )	
7		

### Thermosalinograph (tsg1)

00+019:23:59:46.976 15A16CFC163F8C2C100

Field	Data	Units
1	RVDAS time tag	
2	Seabird hex string (see page 18 for conversion to real units)	

### Fluorometer (flr1)

00+019:23:59:58.061 0 0818 :: 1/19/00 17:23:17 = 0.983 (RAW) 1.2 (C)

Field	Data	Units
1	RVDAS time tag	
2	Marker 0 to 8	
3	4-digit index	

Field	Data	Units
4	Date	mm/dd/yy
5	Time	hh:mm:ss
6	Signal	
7	signal units of measurement	
8	cell temperature	
9	Temperature units	

## pCO<sub>2</sub>

00+021:23:59:43.190 2000021.9992 2382.4 984.2 30.73 50.8 345.9 334.1 -1.70  
-68.046 -144.446 Equil

Field	Data	Units
1	RVDAS time tag	
2	pCO <sub>2</sub> time tag (decimal is fractional time of day)	yyyddd.ttt
3	Raw voltage	mV
4	Barometer	mBar
5	Cell temperature	°C
6	Flow rate	ml/min
7	Concentration	ppm
8	pCO <sub>2</sub> pressure	microAtm
9	Equilibrated temperature	°C
10	Latitude (not collected)	
11	Longitude (not collected)	
12	Flow source (Equil = pCO <sub>2</sub> measurement)	

## Navigational Data

### Seapath GPS (seap)

The Seapath GPS outputs six data strings, four in NMEA format and two in proprietary PSXN format:

- GPZDA
- GPGGA
- GPVTG
- GPHDT
- PSXN, 22
- PSXN, 23

### GPZDA

02+253:00:00:00.772 \$GPZDA,235947.70,09,09,2002,,\*7F

Field	Data	Units
1	RVDAS time tag	
2	\$GPZDA	
3	time	hhmmss.ss
4	Day	dd
5	Month	mm

Field	Data	Units
6	Year	yyyy
7	(empty field)	
8	Checksum	

**GPGGA**

02+253:00:00:00.938

GPGGA,235947.70,6629.239059,S,06827.668899,W,1,07,1.0,11.81,M,,M,,\*6F

Field	Data	Units
1	RVDAS time tag	
2	\$GPGGA	
3	time	hhmmss.ss
4	Latitude	ddmm.mmmmmm
5	N or S for north or south latitude	
6	Longitude	ddmm.mmmmmm
7	E or W for east or west longitude	
8	GPS quality indicator, 0=invalid, 1=GPS SPS, 2=DGPS, 3=PPS, 4=RTK, 5=float RTK, 6=dead reckoning	
9	number of satellites in use (00-99)	
10	HDOP	x.x
9	height above ellipsoid in meters	m.mm
11	M	
12	(empty field)	
13	M	
14	age of DGPS corrections in seconds	s.s
15	DGPS reference station ID (0000-1023)	
16	Checksum	

**GPVTG**

02+253:00:00:00.940 \$GPVTG,19.96,T,,M,4.9,N,,K,A\*39

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	course over ground, degrees true	d.dd
4	T	
5	,	
6	M	
7	speed over ground in knots	k.k
8	N	
9	,	
10	K	
11	Mode	
12	Checksum	

**GPHDT**

02+253:00:00:00.941 \$GPHDT,20.62,T\*23

Field	Data	Units
1	RVDAS time tag	
2	\$GPHDT	
3	Heading, degrees true	d.dd
4	T	
5	Checksum	

**PSXN,22**

02+253:00:00:00.942 \$PSXN,22,0.43,0.43\*39

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	22	
4	gyro calibration value since system start-up in degrees	d.dd
5	short term gyro offset in degrees	d.dd
6	Checksum	

**PSXN,23**

02+253:00:00:02.933 \$PSXN,23,0.47,0.57,20.62,0.03\*0C

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	23	
4	roll in degrees, positive with port side up	d.dd
5	pitch in degrees, positive with bow up	d.dd
6	Heading, degrees true	d.dd
7	heave in meters, positive down	m.mm
8	Checksum	

**Ashtech GPS (3df1)**

The Ashtech GPS outputs three NMEA standard data strings:

- Measurement data (PBN)
- Attitude data (ATT)
- GPS position fix (GGA)

**Measurement data (PBN)**

01+324:00:00:00.064 \$PASHR,PBN,172812.00,2129908.6,-1869076.7,-5694992.4,  
 -063:41.9477,-041:16.0918,00066.2,000.16,002.85,-000.90,08,????,02,01,01,  
 01\*3A

Field	Data	Units
1	RVDAS time tag	
2	\$PASHR	
3	PBN	
4	GPS Time sec. of the week	seconds
5	Station Position: ECEF X	meters
6	Station Position: ECEF Y	meters
7	Station Position: ECEF Z	meters
8	Latitude ( - = South )	deg:min
9	Longitude ( - = West )	deg:min
10	Altitude	meters
11	Velocity in ECEF X	m/sec
12	Velocity in ECEF Y	m/sec
13	Velocity in ECEF Z	m/sec
14	Number of satellites used	
15	Site name	
16	PDOP	

Field	Data	Units
17	HDOP	
18	VDOP	
19	TDOP	

### GPS Position Fix – Geoid/Ellipsoid (GGA)

01+324:00:00:00.323 \$GPGGA,235959.00,6341.9477,S,04116.0918,W,1,08,00.9,  
+00066,M,,M,,\*77

Field	Data	Units
1	RVDAS time tag	
2	\$GPGGA	
3	UTC time at position	hhmmss.ss
4	Latitude	ddmm.mmm
5	North (N) or South (S)	
6	Longitude	ddmm.mmm
7	East (E) or West (W)	
8	GPS quality: (1 = GPS, 2 = DGPS)	
9	Number of GPS satellites used	
10	HDOP	
11	Antenna height	meters
12	M for Meters	
13	Geoidal height (no data in the sample string)	meters
14	M for meters	
15	Age of diff. GPS data (no data in the sample string)	
16	Differential reference station ID (no data in the sample string)	
17	Checksum (no delimiter before this field)	

### Attitude Data (ATT)

01+324:00:00:00.845 \$PASHR,ATT,172813.0,137.88,+000.52,-001.41,0.0029,  
0.0254,0\*2F

Field	Data	Units
1	RVDAS Time tag	
2	\$PASHR	
3	ATT	
4	GPS Time sec. Of the week	seconds
5	Heading (rel. to true North)	degrees
6	Pitch	degrees
7	Roll	degrees
8	Measurement RMS error	meters
9	Baseline RMS error	meters
10	Attitude reset flag	

### Trimble GPS (PCOD)

The Trimble GPS outputs three NMEA standard data strings:

- Position fix (GGA)
- Latitude / longitude (GLL),
- Track and ground speed (VTG)

### GGA: GPS Position Fix – Geoid/Ellipsoid

01+319:00:04:11.193 \$GPGGA,000410.312,6227.8068,S,06043.6738,W,1,06,1.0,  
031.9,M,-017.4,M,,\*49

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGGA	
3	UTC time at position	hhmmss.sss
4	Latitude	ddmm.mmm
5	North (N) or South (S)	
6	Longitude	ddmm.mmm
7	East (E) or West (W)	
8	GPS quality: 0 = Fix not available or invalid 1 = GPS, SPS mode, fix valid 2 = DGPS (differential GPS), SPS mode, fix valid 3 = P-CODE PPS mode, fix valid	
9	Number of GPS satellites used	
10	HDOP (horizontal dilution of precision)	
11	Antenna height	meters
12	M for meters	
13	Geoidal height	meters
14	M for meters	
15	Age of differential GPS data (no data in the sample string)	
16	Differential reference station ID (no data in the sample string)	
17	Checksum (no delimiter before this field)	

### GLL: GPS Latitude/Longitude

01+319:00:04:11.272 \$GPGLL,6227.8068,S,06043.6738,W,000410.312,A\*32

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGLL	
3	Latitude	degrees
4	North or South	
5	Longitude	degrees
6	East or West	
7	UTC of position	hhmmss.sss
8	Status of data (A = valid)	
9	Checksum	

### VTG: GPS Track and Ground Speed

01+319:00:04:11.273 \$GPVTG,138.8,T,126.0,M,000.0,N,000.0,K\*49

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	Heading	degrees
4	Degrees true (T)	
5	Heading	degrees
6	Degrees magnetic (M)	
7	Ship speed	knots
8	N = knots	
9	Speed	km/hr
10	K = km per hour	
11	Checksum	

**Gyro Compass (gyr1)**

00+019:23:59:59.952 \$HEHRC 25034,-020 \*73

Field	Data	Units
1	RVDAS time tag	
2	\$HEHRC	
3	Heading XXXXX = ddd.dd	degrees
4	Rate of change SYYY S = +/-, YYY = r.rr	
5	Checksum	

**ADCP Course (adcp)**

00+019:23:59:59.099 \$PUHAW,UVH,-1.48,-0.51,250.6

Field	Data	Units
1	RVDAS time tag	
2	\$PUHAW	
3	UVH (E-W, N-S, Heading)	
4	Ship Speed relative to reference layer, east vector	knots
5	Ship Speed relative to reference layer, north vector	knots
6	Ship heading	degrees

**Sound Velocity Probe (svp1)**

00+348:01:59:52.128 1539.40

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

**Process****pCO<sub>2</sub>-merged**

00+346:23:58:20.672 2000346.9991 2398.4 1008.4 0.01 45.4 350.3 342.6  
 15.77 Equil -43.6826 173.1997 15.51 33.90 0.33 5.28 9.05 1007.57 40.0  
 14.87 182.44

Field	Data	Units
1	RVDAS time tag	
2	PCO <sub>2</sub> time tag (decimal is time of day)	yyyddd.ttt
3	Raw voltage	mV
4	Barometer	mB
5	Cell temperature	°C
6	Flow rate	cm <sup>3</sup> /min
7	Concentration	ppm
8	PCO <sub>2</sub> pressure	microAtm
9	Equilibrated temperature	°C
10	Flow Source (Equil = pCO <sub>2</sub> measurement)	
11	RVDAS latitude	degrees
12	RVDAS longitude	degrees
13	TSG external temperature	°C
14	TSG salinity	PSU
15	TSG fluorometry	V

Field	Data	Units
16	RVDAS true wind speed	m/s
17	RVDAS true wind direction	degrees
18	Barometric Pressure	mBars
19	Uncontaminated seawater pump flow rate	l/min
20	Speed over ground	knots
21	Course made good	degrees

**tsqfl**

00+075:00:00:04.467 -01.488 -01.720 02.6783 33.63748 1.002442 0.002442

Field	Data	Units
1	RVDAS time tag	
2	Internal water temperature	°C
3	Sea Surface Temperature	°C
4	Conductivity	μSiemens/m
5	Salinity	PSU
6	Fluorometry	V
7	Transmissivity	V

## Calculations

The file *rvdascal.txt* located in the `/reports` directory contains the calibration factors for shipboard instruments. This was the file used by the RVDAS processing software.

### TSG

Raw TSG data is stored as a 20 byte (character) long hex string

Bytes	Data
1-4	Sensor Temperature
5-8	Conductivity
9-14	Remote Temperature
15-17	Fluorometer voltage
18-20	Transmissometer voltage

The coefficients for temperature and conductivity sensors can be found the *rvdascal.txt* file and on the calibrations sheets in the appendix.

#### Calculating Temperature – ITS-90

```
T = decimal equivalent of bytes 1-4
Temperature Frequency:  f = T/19 + 2100
Temperature = 1/{g + h[ln(f0/f)] + i[ln2(f0/f)] + j[ln3(f0/f)]} -
273.15 (°C)
```

#### Calculating Conductivity – ITS-90

```
C = decimal equivalent of bytes 5-8
Conductivity Frequency f = sqrt(C*2100+6250000)
Conductivity = (g + hf2 + if3 + jf4)/[10(1 + δt + εp)]
(siemens/meter)
t = temperature (°C); p = pressure (decibars); δ = Ctcor; ε =
CPcor
```

#### Calculating Fluorometry Voltage from the TSG

```
f = decimal equivalent of bytes 15-17
Fluorometry Voltage = f/819
```

#### Calculating Transmittance

```
Vdark = 0.058 V
Vref = 4.765 V
t = decimal equivalent of bytes 18 - 20
Transmissometer Voltage (Vsignal) = t/819
% Transmittance = (Vsignal - Vdark) / (Vref - Vdark)
```

### PAR

```
raw data = mV
calibration scale = 6.08 V/(μEinstiens/cm2sec)
offset (Vdark) = 0.3 mV
(raw mV - Vdark)/scale x 104 cm2/m2 x 10-3 V/mV = μEinstiens/m2sec
or
(data mV - 0.3 mV) x 1.65 (μEinstiens/m2sec)/mV =
μEinstiens/m2sec
```

**PIR**

raw data = mV

calibration scale =  $4.13 \times 10^{-6} \text{ V/(W/m}^2\text{)}$

data mV / (scale  $\times 10^3 \text{ mV/V}$ ) =  $\text{W/m}^2$

or

data mV  $\times 242.1 (\text{W/m}^2)/\text{mV} = \text{W/m}^2$

**PSP**

raw data = mV

calibration scale =  $8.28 \times 10^{-6} \text{ V/(W/m}^2\text{)}$

data mV / (scale  $\times 10^3 \text{ mV/V}$ ) =  $\text{W/m}^2$

or

data mV  $\times 120.7 (\text{W/m}^2)/\text{V} = \text{W/m}^2$

This section lists problems with acquisition noted during this cruise including instrument failures, data acquisition system failures and any other factor affecting this data set. The format is ddd:hh:mm (ddd is year-day, hh is hour, and mm is minute). Times are reported in GMT.

[illegible]

## Appendix: Sensors and Calibrations

### NBP0305A Sensors:

#### *Shipboard Sensors*

Sensor	Description	Serial #	Last Calibration Date	Status
<b>Meteorology &amp; Radiometers</b>				
Port Anemometer	RM Young 5106	WM46262	11/25/03	
Stbd Anemometer	RM Young 5106	WM51143	6/15/03	
Barometer	RM Young 61201	01705	07/04/03	
Air Temp/Rel. Hum.	RM Young 41372LC	06135	04/09/03	
PIR (Pyrgometer)	Eppler PIR	32845F3	7/03/03	
PSP (Pyranometer)	Eppler PSP	32850F3	7/03/03	
Mast PAR	BSI QSR-240	6356	02/03/03	
Mast PAR	BSI QSR-240	6357	06/24/03	
GUV	BSI GUUV-2511	2511020314	6/05/03	
PUV	BSI PUV-2500	2500020314	6/05/03	
PRR (surface)	BSI PRR-610	9696	6/4/03	Not used
PRR (underwater)	BSI PRR-600	9695	6/12/03	Not used
<b>Underway</b>				
TSG	SeaBird SBE21	214857-0857	2/11/03	Not used
TSG	SeaBird SBE21	218091-1390	5/29/03	
TSG Remote Temp	SeaBird 3-01/S	032593	02/06/03	
Fluorometer	Turner 10-AU-005 Lamp: daylight 10-045; ref. filter: 10-032, em. filter: 10-051, ex. filter: 10-050	5651 FRTD	Not	
Transmissometer	WET Labs C-Star	CST-422PR	10/15/03	
Bathymetry	Simrad EK500	3001	11/1/95	
Bathymetry	ODEC Bathy 2000			
<b>Other</b>				
P-Code GPS	Trimble 20636-00 (SM)	0220035116	Key expired	
Attitude GPS	Ashtech ADU2	700273F2114 FW 7B13-D1-C21	N/A	
Seapath GPS	Kongsberg Seatex Seapath 200	2253	N/A	

**CTD**

Sensor	Description	Serial #	Last Calibration Date	Status
CTD Fish	SBE-9+	09P10716-0377	6/3/03	
CTD Pressure Sensor	410K-105	58949	6/3/03	
Temperature	Primary	1238	7/1/03	
Temperature	Secondary	2168	7/1/03	
Conductivity	Primary	41143	7/1/03	
Conductivity	Secondary	40926	5/30/03	
Dissolved Oxygen	SBE 43	0150	6/18/03	Not Used
Fluorometer	Chelsea Mk III Aquatracka	88080	2/23/03	
Transmissometer	Wetlabs CST-397DR	CST-397DR	2/25/03	

## Calibrations

The following pages are replicas of current calibration sheets for the sensors used during this cruise.

### CTD

#### Pressure Sensor

0305N377CON.txt

S/N: Pressure Sensor-Fish  
58949-0377  
Cal Date: 03-June-2003

T1: 2.998410e+01  
T2: -2.451935e-04  
T3: 3.711743e-06  
T4: 2.102236e-09  
T5: 0.000000e+00

C1: -4.839620e+04  
C2: 3.519636e-01  
C3: 8.922267e-03

D1: 3.977913e-02  
D2: 3.026373e-05  
AD590M: 1.250000e-02  
AD590B: -1.000000e+01

Slope: 1.00000000  
Offset: 0.00000

Scripps  
Pressure  
Sensor  
Calibration

**Primary Temperature Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1238  
CALIBRATION DATE: 01-Jul-03SBE3 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.82469840e-003$   
 $h = 6.70789172e-004$   
 $i = 2.57160859e-005$   
 $j = 2.05651777e-006$   
 $f_0 = 1000.0$

## ITS-68 COEFFICIENTS


$a = 3.68120926e-003$   
 $b = 5.97985016e-004$   
 $c = 1.45614054e-005$   
 $d = 2.05791731e-006$   
 $f_0 = 6124.972$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.4997	6124.972	-1.4998	-0.00007
1.0003	6479.254	1.0004	0.00011
4.5003	6999.686	4.5004	0.00005
8.0004	7549.402	8.0003	-0.00008
11.5004	8129.181	11.5003	-0.00009
15.0003	8739.777	15.0003	0.00004
18.5003	9381.914	18.5004	0.00007
22.0004	10056.291	22.0004	-0.00002
25.5004	10763.583	25.5004	-0.00004
29.0003	11504.444	29.0003	0.00004
32.5004	12279.509	32.5004	-0.00002

$$\text{Temperature ITS-90} = 1 / \{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature ITS-68} = 1 / \{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 \times T_{90}$  (-2 to 35  $^\circ\text{C}$ )

Residual = instrument temperature - bath temperature

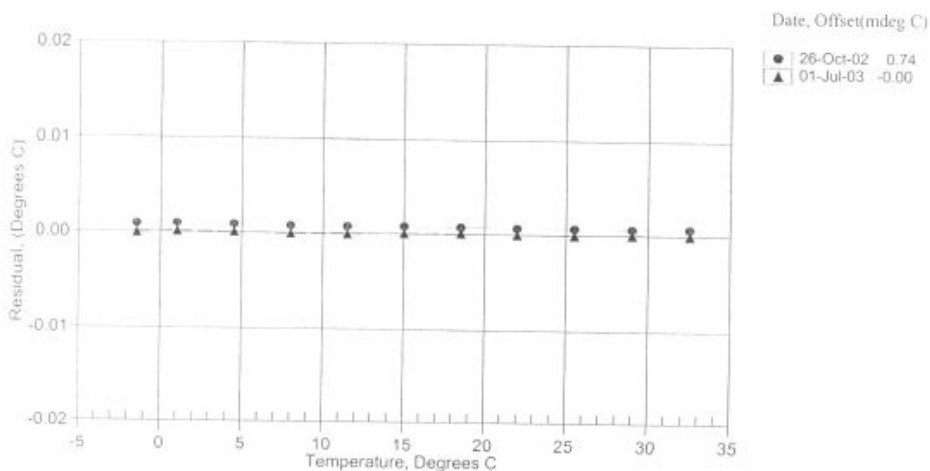

**Secondary Temperature Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2168  
CALIBRATION DATE: 01-Jul-03SBE3 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.35104308e-003$   
 $h = 6.44232035e-004$   
 $i = 2.36446513e-005$   
 $j = 2.26277029e-006$   
 $f0 = 1000.0$

## ITS-68 COEFFICIENTS


$a = 3.68120869e-003$   
 $b = 6.01288629e-004$   
 $c = 1.63543995e-005$   
 $d = 2.26434101e-006$   
 $f0 = 2938.794$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.4997	2938.794	-1.4997	-0.00003
1.0003	3107.840	1.0004	0.00006
4.5003	3356.178	4.5003	0.00002
8.0004	3618.501	8.0003	-0.00008
11.5004	3895.187	11.5004	-0.00004
15.0003	4186.597	15.0004	0.00005
18.5003	4493.093	18.5004	0.00007
22.0004	4815.016	22.0004	-0.00002
25.5004	5152.692	25.5003	-0.00007
29.0003	5506.450	29.0003	0.00002
32.5004	5876.603	32.5004	0.00001

$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS:  $T_{90}$  is assumed to be  $1.00024 \cdot T_{90}$  (-2 to 35  $^\circ\text{C}$ )

Residual = instrument temperature - bath temperature

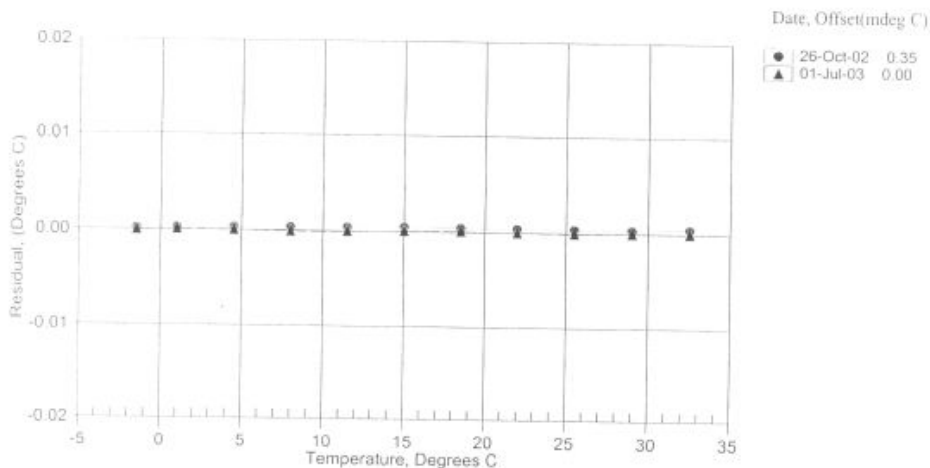

**Dissolved Oxygen Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0150  
CALIBRATION DATE: 18-Jun-03p

## SBE 43 OXYGEN CALIBRATION DATA

## COEFFICIENTS

Soc = 0.4380

Soc = 0.0000

Voffset = -0.4841

TCor = 0.0015

PCor = 1.350e-04

BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL. PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.63	5.00	0.04	0.898	1.63	-0.00
1.64	25.00	0.03	1.109	1.64	-0.00
1.49	25.00	0.03	1.434	1.49	0.00
2.52	5.00	0.04	1.123	2.52	-0.00
3.35	25.00	0.03	1.765	3.36	0.01
3.39	5.00	0.04	1.345	3.39	0.00
5.08	25.00	0.03	2.421	5.08	-0.00
5.20	5.00	0.04	1.804	5.20	0.00
6.67	5.00	0.04	2.179	6.67	0.00
6.79	25.00	0.03	3.074	6.79	-0.00


oxygen (ml/l) = (Soc \* (V + Voffset)) \* exp(Tcor \* T) \* Oxsat(T,S) \* exp(PCor \* P)

V = voltage output from SBE43, T = ocean temperature [deg C]

S = ocean salinity [PSU] from CTD, P = ocean pressure [dbar] from CTD

Oxsat(T,S) = oxygen saturation [ml/l]

Residual = instrument oxygen - bath oxygen

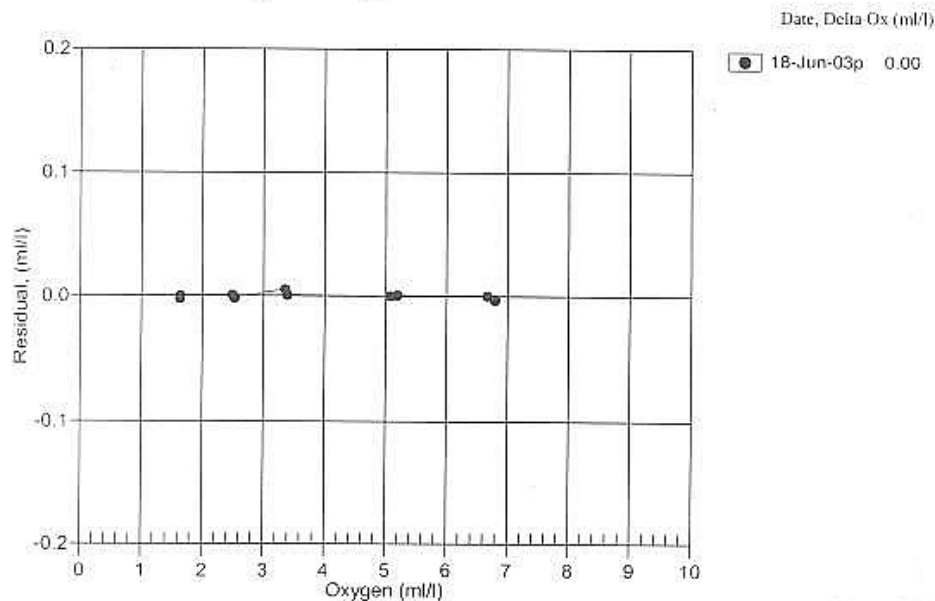

**Fluorometer****CERTIFICATE OF CALIBRATION**

Date of issue      23<sup>rd</sup> February 2003

Description      Mk III Aquatracka (Chlorophyll-a)

Serial Number      088080

**Chelsea  
Technologies  
Group**

55 Central Avenue  
West Molesey  
Surrey KT8 2QZ  
United Kingdom  
Tel: +44 (0)20 8481 9000  
Fax: +44 (0)20 8941 9319  
sales@chelsea.co.uk  
www.chelsea.co.uk

**REPORT**

The fluorimeter was exposed to various concentrations of Chlorophyll-a dissolved in acetone in addition to pure water and pure acetone. The following formula was derived from the readings to relate instrument output to chlorophyll-a concentration.

$$\text{Conc.} = (0.0157 \times 10^{\text{Output}}) - 0.037$$

Where:-

conc. = fluorophor concentration in µg/l

Output = Aquatracka output in volts

The above formula can be used in the range 0 - 100 microgrammes per litre to an uncertainty of 0.02 microgrammes per litre plus 8% of value.

**Notes**

The above formula has been derived using Chlorophyll-a dissolved in acetone. No guarantee is given as to the performance of the instrument to biologically active chlorophyll in sea-water.

The zero offset has been determined in the laboratory using purified water from a reverse osmosis/ion exchange column. It is possible that purer water may be found in clean deep ocean conditions. Under these conditions, the offset shown in the above formula should be replaced by the antilogarithm of the Aquatracka output in the purest water found, multiplied by the scale factor.

**Group Companies**

Chelsea Technologies Ltd  
Chelsea Instruments Ltd  
Chelsea Environmental Ltd

Serial number 088080

Page 1 of 2

Fluorimeter calibration readings

Ambient temperature 20°C

Output for detector mechanically blanked 0.296 Volts

Output for pure water 0.375 Volts

chlorophyll concentration in acetone (µg/l)	Output (volts)
Acetone (pure)	0.3297
0.1038	0.9715
0.3114	1.3278
1.038	1.8172
3.10362	2.3170
10.2762	2.8166
30.2058	3.2842
94.3542	3.7660

The uncertainty of the chlorophyll concentration is estimated not to exceed 3%. The uncertainty of output voltage measurement is estimated not to exceed 2mV.

Signed

Christina

Date

23.02.03

**Transmissometer**

## Wetlabs C-Star Transmissometer N.B.Palmer Onboard Calibration Sheet

**Calibration Date:** 02/25/03

**Serial Number:** CST-397DR

**Technician:** Wetlabs Job #0009009 (from Wetlabs Cal Sheet)

Use the following table to enter voltages when performing an annual calibration of the instrument:

$Y_0 = V_d$	0.059	Voltage Blocked
$A_0 = V_{air}$	4.818	Voltage in air
$W_0 = V_{ref}$	4.778	Voltage in pure filtered H <sub>2</sub> O from the Nanopure system.
Cal. Temp of Water	19.4	Temperature of the water during calibration. (Centigrade)
Ambient Temp	20.5	Air temperature during the calibration. (Centigrade)

The following equation is used by RVDas to obtain % of Transmittance:

$$\% \text{ Transmission} = 100\% * (V_{sig} - V_d) / (V_{ref} - V_d) \quad V_{sig} = \text{Signal Voltage at any point in time.}$$

Use the following table to enter measured voltages when putting the instrument in use:

**Note:** Use the system that the instrument is being installed in to measure the voltage.  
(i.e., CTD: Use the CTD Deck unit and read the voltage on the CTD Computer with the system on.)

*Make sure the lenses are clean and dry!*

**Date:**

**Technician:**

**System:**

	Value	Comments
$Y_1 = V_{dark}$ (current)		Current measured blocked voltage.
$A_1 = V_{air}$ (current)		Current measured voltage in air.
$T_w$	100%	%Transmission in pure water.

Use the following equations to obtain the M and B constants for Seasave for both the CTD and Thermosalinagraph:

(Select Chelsea/Seatech/ Wetlab CStar in Seasave for Windows or Transmissometer in Seacon for DOS).  
(Do NOT select Beam Transmissometer or WetLab AC3)

$$M = (T_w / W_0) * (A_0 - Y_0) / (A_1 - Y_1) \quad B = -M Y_1$$

$$M = (100 / \quad) * ( \quad - \quad ) / ( \quad - \quad ) \quad B =$$

$$M = \quad \quad B =$$

$$\text{Path Length (M)} = 0.250$$

**Primary Conductivity Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1143  
CALIBRATION DATE: 01-Jul-03SBE4 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## GHIJ COEFFICIENTS


$g = -4.17024877e+000$   
 $h = 5.32455622e-001$   
 $i = 7.38502005e-005$   
 $j = 2.41699148e-005$   
 $CPcor = -9.5700e-008$  (nominal)  
 $CTcor = 3.2500e-006$  (nominal)

## ABCDM COEFFICIENTS

$a = 4.79564475e-005$   
 $b = 5.32570279e-001$   
 $c = -4.17040491e+000$   
 $d = -8.18733405e-005$   
 $m = 3.8$   
 $CPcor = -9.5700e-008$  (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.79755	0.00000	0.00000
-1.0003	34.7760	2.80161	7.76012	2.80162	0.00001
0.9997	34.7766	2.97287	7.96321	2.97286	-0.00001
14.9997	34.7771	4.26728	9.35513	4.26729	0.00001
18.4997	34.7777	4.61377	9.69332	4.61374	-0.00003
28.9997	34.7755	5.69636	10.68019	5.69641	0.00006
32.4997	34.7703	6.06884	10.99877	6.06881	-0.00004

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p) \text{ Siemens/meter}$$
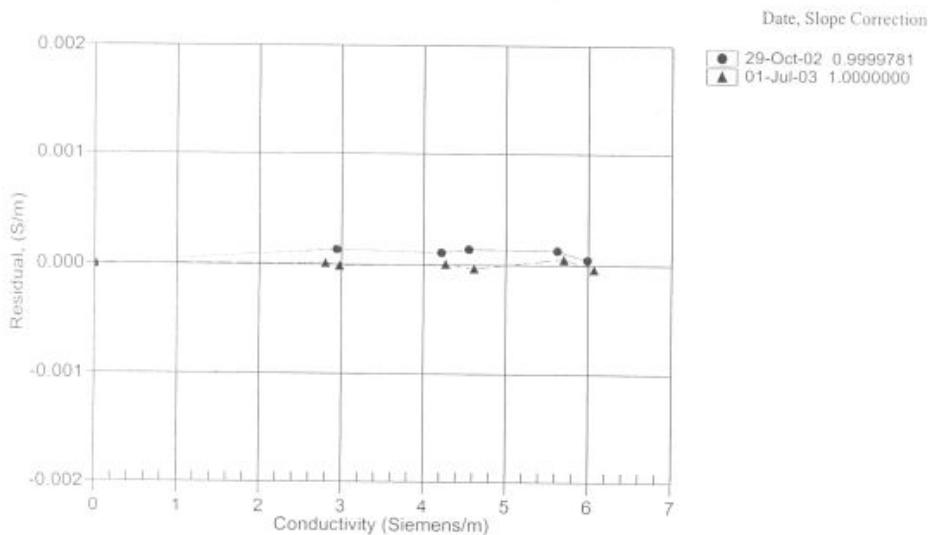
$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10(1 + \epsilon p)] \text{ Siemens/meter}$$
 $t = \text{temperature}[^{\circ}\text{C}]; p = \text{pressure}[\text{decibars}]; \delta = CTcor; \epsilon = CPcor;$ 
 $\text{Residual} = (\text{instrument conductivity} - \text{bath conductivity}) \text{ using } g, h, i, j \text{ coefficients}$ 


## Secondary Conductivity Sensor

### SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0926  
CALIBRATION DATE: 30-May-03SBE4 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## GHJ COEFFICIENTS

$g = -4.03464395e+000$   
 $h = 5.28224814e-001$   
 $i = -5.23670332e-004$   
 $j = 5.47318613e-005$   
 $CPcor = -9.5700e-008$  (nominal)  
 $CTcor = 3.2500e-006$  (nominal)

## ABCDM COEFFICIENTS


$a = 1.89828871e-006$   
 $b = 5.26490908e-001$   
 $c = -4.02946953e+000$   
 $d = -8.60725149e-005$   
 $m = 5.0$   
 $CPcor = -9.5700e-008$  (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.76641	0.00000	0.00000
-1.0003	34.6190	2.79013	7.78116	2.79015	0.00002
0.9997	34.6197	2.96073	7.98574	2.96072	-0.00001
14.9997	34.6202	4.25007	9.38705	4.25005	-0.00001
18.4997	34.6205	4.59516	9.72731	4.59515	-0.00001
28.9997	34.6199	5.67373	10.71976	5.67377	0.00004
32.4998	34.6170	6.04513	11.04024	6.04510	-0.00003

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p) \text{ Siemens/meter}$$

$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10(1 + \epsilon p) \text{ Siemens/meter}]$$

$$t = \text{temperature}[^{\circ}\text{C}]; p = \text{pressure[decibars]}; \delta = CTcor; \epsilon = CPcor;$$
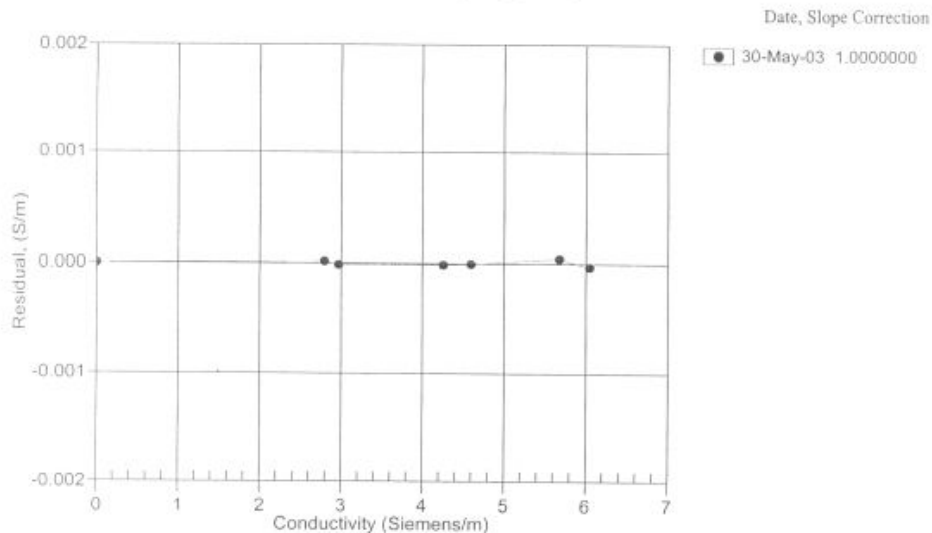
$$\text{Residual} = (\text{instrument conductivity} - \text{bath conductivity}) \text{ using } g, h, i, j \text{ coefficients}$$


**Meteorology System****Anemometer (Port)****RM Young Anemometer Calibration, Model 05106**

S/N: 45262

Date: 25-Feb-03

Cal'd By: Bruce Felix

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.0	0.0	0
200	0.98	0.9	0.1	1.904
500	2.45	2.3	0.2	4.76
1000	4.90	4.8	0.1	9.52
1500	7.35	7.3	0.0	14.28
2000	9.80	9.8	0.0	19.04
3000	14.70	14.8	-0.1	28.56
4000	19.60	19.8	-0.2	38.08
5000	24.50	24.8	-0.3	47.6
6000	29.40	29.8	-0.4	57.12
7000	34.30	34.7	-0.4	66.64
8000	39.20	39.7	-0.5	76.16
9000	44.10	44.7	-0.6	85.68
10000	49.00	49.6	-0.6	95.2
12000	58.80	59.4	-0.6	114.24

Direction	Measured Direction	Delta Direction
0	0	0
30	28.5	1.5
60	59	1
90	90	0
120	120	0
150	149	1
180	179	1
210	209	1
240	240	0
270	269.5	0.5
300	300	0
330	330	0
0	0	0

**Note:** Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.0	0.0
200	0.98	0.9	0.1
500	2.45	2.3	0.2
1000	4.90	4.8	0.1
1500	7.35	7.3	0.0
2000	9.80	9.8	0.0
3000	14.70	14.8	-0.1
4000	19.60	19.8	-0.2
5000	24.50	24.8	-0.3
6000	29.40	29.8	-0.4
7000	34.30	34.7	-0.4
8000	39.20	39.7	-0.5
9000	44.10	44.7	-0.6
10000	49.00	49.7	-0.6
12000	58.80	59.5	-0.7

**Caution:** Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm? ☒ Yes  
 Wind Direction Threshold < 30 gm? ☒ Yes

**Additional Comments**

**Note:** Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

**Anemometer (Starboard)****RM Young Anemometer Calibration, Model 05106**

S/N: 51143

Date: 15-Jun-03

Cal'd By: S. Blackman

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	knots
0	0.00	0.0	0.0	0.0
200	0.98	0.9	0.1	1.9
500	2.45	2.3	0.2	4.8
1000	4.90	4.8	0.1	9.5
1500	7.35	7.4	-0.1	14.3
2000	9.80	9.8	0.0	19.0
3000	14.70	14.8	-0.1	28.6
4000	19.60	19.8	-0.2	38.1
5000	24.50	24.8	-0.3	47.6
6000	29.40	29.7	-0.3	57.1
7000	34.30	34.7	-0.4	66.6
8000	39.20	39.7	-0.5	76.2
9000	44.10	44.7	-0.6	85.7
10000	49.00	49.6	-0.6	95.2
12000	58.80	59.5	-0.7	114.2

Direction	Measured Direction	Delta Direction
0	0	0
30	29	1
60	59	1
90	89	1
120	120	0
150	150	0
180	180	0
210	210	0
240	242	-2
270	273	-3
300	302	-2
330	332	-2
0	0	0

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.1	-0.1
200	0.98	0.9	0.1
500	2.45	2.3	0.2
1000	4.90	4.8	0.1
1500	7.35	7.3	0.0
2000	9.80	9.8	0.0
3000	14.70	14.8	-0.1
4000	19.60	19.8	-0.2
5000	24.50	24.8	-0.3
6000	29.40	29.8	-0.4
7000	34.30	34.7	-0.4
8000	39.20	39.7	-0.5
9000	44.10	44.7	-0.6
10000	49.00	49.6	-0.6
12000	58.80	59.5	-0.7

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm?

Wind Direction Threshold < 30 gm?

**Additional Comments**

This instrument does not appear to have been used. It's new cal date should start with it's installation.

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

**PIR****THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave. P.O. Box 419, Newport, RI 02840 USA

Telephone 401-847-1020

Fax 401-847-1031

Email: eplab@mail.bbsnet.com

Internet: www.eppleylab.com

Scientific Instruments  
for Precision Measurements  
Since 1911**STANDARDIZATION OF  
EPPLEY PRECISION INFRARED RADIOMETER  
Model PIR**

Serial Number: 32845F3

Resistance: 739  $\Omega$  at 23  $^{\circ}\text{C}$   
Temperature Compensation Range: -20 to 40  $^{\circ}\text{C}$ 

This pyrometer has been compared with Precision Infrared Radiometer, Serial Number 29326F3 in Eppley's Blackbody Calibration System under radiation intensities of approximately 200 watts meter<sup>-2</sup> and an average ambient temperature of 24  $^{\circ}\text{C}$ .

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$4.14 \times 10^{-8} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 700 watts meter<sup>-2</sup>. This radiometer is linear to within  $\pm 1.0\%$  up to this intensity.

The calibration of this instrument is traceable to the International Practical Temperature Scale (IPTS) through a precision low-temperature blackbody.

Shipped to:  
Raytheon Polar Services  
Port Hueneme, CA

Date of Test: June 9, 2003

In Charge of Test: *R.T. Gorman*

S.O. Number: 39471  
Date: July 3, 2003

Reviewed by: *Thomas D. Kuh*

Remarks:

**PSP****Biospherical Instruments Inc.**

## CALIBRATION CERTIFICATE

Calibration Date: 2/3/03  
 Model Number: QSR-240 *Must PAR*  
 Serial Number: 6356  
 Operator: TPC  
 Standard Lamp: 98700(5/19/01)  
 Probe Excitation Voltage Range: 5 to 18 VDC(+)  
 Output Polarity: Positive

Probe Conditions at Calibration(in air):

Calibration Voltage: 6 VDC(+)  
 Probe Current: 1.2 mA

Probe Output Voltage:

Probe Illuminated: 92.4 mV  
 Probe Dark: 0.4 mV  
 Probe Net Response: 92.0 mV

Corrected Lamp Output:

Output In Air (same condition as calibration):

9.14E+15 quanta/cm<sup>2</sup>sec  
0.015 uE/cm<sup>2</sup>sec

Calibration Factor:

(To calculate irradiance, divide the net voltage reading in Volts by this value.)

Dry: 1.01E-17 V/(quanta/cm<sup>2</sup>sec)  
6.06E+00 V/(uE/cm<sup>2</sup>sec)

## Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with alcohol.
4. Calibration was performed with customer cable, when available.

:240R 05/24/95

**PAR****THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA

Telephone: 401-847-1020

Fax: 401-847-1031

Email: eplab@mail.bbsnet.com

Internet: www.eppleylab.com

Scientific Instruments  
for Precision Measurements  
Since 1917

**STANDARDIZATION  
OF  
EPPLEY PRECISION SPECTRAL PYRANOMETER  
Model PSP**

Serial Number: **32850F3**

Resistance: 706  $\Omega$  at 23  $^{\circ}\text{C}$   
 Temperature Compensation Range: -20 to 40  $^{\circ}\text{C}$

This radiometer has been compared with Standard Precision Spectral Pyranometer, Serial Number 21231F3 in Eppley's Integrating Hemisphere under radiation intensities of approximately 700 watts meter<sup>-2</sup> (roughly one-half a solar constant). The adopted calibration temperature is 25  $^{\circ}\text{C}$ .

As a result of a series of comparisons, it has been found to have a sensitivity of:

8.12  $\times 10^{-6}$  volts/watts meter<sup>-2</sup>

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 1400 watts meter<sup>-2</sup>. This radiometer is linear to within  $\pm 0.5\%$  up to this intensity.

The calibration of this instrument is traceable to standard self-calibrating cavity pyrheliometers in terms of the Systems Internationale des Unites (SI units), which participated in the Ninth International Pyrheliometric Comparisons (IPC IX) at Davos, Switzerland in September-October 2000.

Useful conversion facts: 1 cal cm<sup>-2</sup> min<sup>-1</sup> = 697.3 watts meter<sup>-2</sup>  
 1 BTU/ft<sup>2</sup>-hr<sup>-1</sup> = 3.153 watts meter<sup>-2</sup>

Shipped to:  
Raytheon Services  
Port Hueneme, CA

Date of Test: July 3, 2003

In Charge of Test: *R.T. Egan*

S.O. Number: 59471  
Date: July 3, 2003

Reviewed by: *Thomas D. Kuk*

Remarks: Sensitivity before repainting 7.97

Installed 11/2/03 03:03 GMT

# Biospherical Instruments Inc.

## CALIBRATION CERTIFICATE

Calibration Date 6/24/03  
 Model Number QSR-240  
 Serial Number 6357  
 Operator TPC  
 Standard Lamp 98700(5/19/01)  
 Probe Excitation Voltage Range: 5 to 18 VDC(+) 5  
 Output Polarity: Positive

### Probe Conditions at Calibration (in air):

Calibration Voltage: 5 VDC(+) 5  
 Probe Current: 7.1 mA

### Probe Output Voltage:

Probe Illuminated 94.7 mV  
 Probe Dark 2.1 mV  
 Probe Net Response 92.6 mV

### Corrected Lamp Output:

Output In Air (same condition as calibration):

9.14E+15 quanta/cm<sup>2</sup>sec  
0.015 uE/cm<sup>2</sup>sec

### Calibration Factor:

(To calculate irradiance, divide the net voltage reading in Volts by this value.)

Dry: 1.01E-17 V/(quanta/cm<sup>2</sup>sec)  
6.10E+00 V/(uE/cm<sup>2</sup>sec)

### Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with alcohol.
4. Calibration was performed with customer cable, when available.

QSR240R 05/24/95

## TSG Calibration Files

## Underway Conductivity Sensor

Installed 11/1/03 21:40 GMT

## SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1390  
CALIBRATION DATE: 29-May-03SBE21 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## GHIJ COEFFICIENTS

$g = -3.92868160e+000$   
 $h = 4.69806858e-001$   
 $i = 7.64098134e-004$   
 $j = -1.60788378e-005$   
 $CPcor = -9.5700e-008$  (nominal)  
 $CTcor = 3.2500e-006$  (nominal)


## ABCDM COEFFICIENTS

$a = 3.67483151e-002$   
 $b = 4.29412267e-001$   
 $c = -3.91316767e+000$   
 $d = -9.02523180e-005$   
 $m = 2.1$   
 $CPcor = -9.5700e-008$  (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2.88542	0.00000	0.00000
1.0000	34.8296	2.97699	8.42198	2.97701	0.00001
4.4999	34.8298	3.28586	8.79780	3.28585	-0.00001
15.0001	34.8286	4.27297	9.90293	4.27297	-0.00000
18.4998	34.8281	4.61975	10.26266	4.61971	-0.00003
24.0000	34.8272	5.18007	10.81853	5.18010	0.00003
28.9999	34.8259	5.70370	11.31305	5.70372	0.00002
32.5000	34.8235	6.07710	11.65274	6.07708	-0.00002

Conductivity =  $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$  Siemens/meterConductivity =  $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$  Siemens/meter $t$  = temperature[°C];  $p$  = pressure[decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;Residual = (instrument conductivity - bath conductivity) using  $g, h, i, j$  coefficients

Date, Slope Correcti

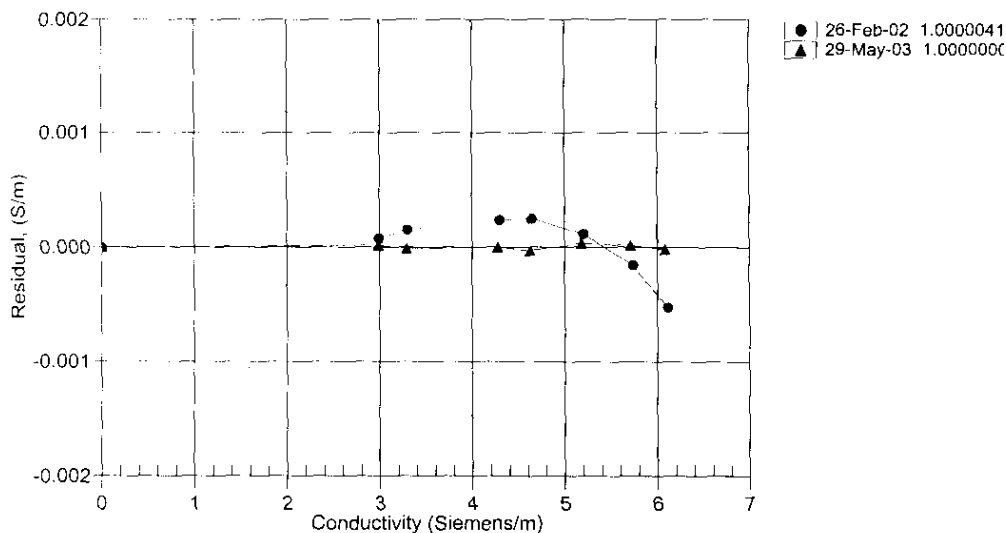

**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington 98005 USA  
 Phone: (425) 643 - 9866 Fax: (425) 643 - 9954 Internet: seabird@seabird.com

SENSOR SERIAL NUMBER = 857  
 CALIBRATION DATE: 11-Feb-03

CONDUCTIVITY CALIBRATION DATA  
 PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

**GHI COEFFICIENTS**

g = -3.88487313e+00  
 h = 4.63101992e-01  
 i = 1.34441099e-03  
 j = -3.93800080e-05  
 CPcor = -9.57e-08 (nominal)  
 CTcor = 3.25e-06 (nominal)

**ABCDM COEFFICIENTS**

a = 4.56144948e-02  
 b = 4.15067913e-01  
 c = -3.87643249e+00  
 d = -1.63462167e-04  
 m = 2.1  
 CPcor = -9.57e-08 (nominal)


BATH TEMP (ITS-90 °C)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2.88531	0.00000	0.00000
1.0000	35.0014	2.99027	8.46371	2.99021	-0.00006
4.4999	35.0000	3.30033	8.84134	3.30035	0.00002
15.0000	34.9951	4.29122	9.95142	4.29131	0.00009
18.5001	34.9938	4.63937	10.31285	4.63946	0.00009
24.0001	34.9932	5.20202	10.87115	5.20186	-0.00016
29.0001	34.9903	5.72761	11.36808	5.72753	-0.00008
32.5000	34.9866	6.10232	11.70953	6.10242	0.00010

Conductivity =  $(g + hT^2 + iT^3 + jT^4) / [10(1 + \delta T + \epsilon p)]$  Siemens/meter

Conductivity =  $(af^n + bf^2 + c + dt) / [10(1 + \epsilon p)]$  Siemens/meter

T = temperature [deg C]; p = pressure [decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

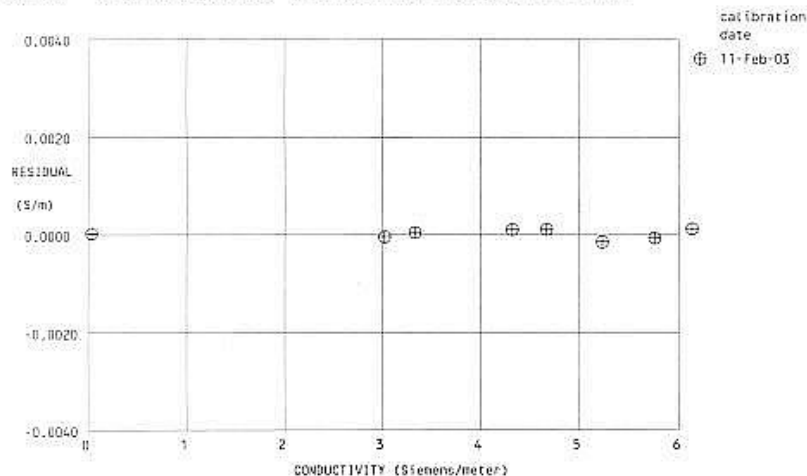

**Underway Temperature Sensor**

installed 11/5/03 21:40 GMT

**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1390  
CALIBRATION DATE: 29-May-03SBE21 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.21019024e-003$   
 $h = 5.94640281e-004$   
 $i = 4.44891723e-006$   
 $j = -1.86469051e-006$   
 $f0 = 1000.0$

## ITS-68 COEFFICIENTS


$a = 3.64763709e-003$   
 $b = 5.81167551e-004$   
 $c = 9.81916346e-006$   
 $d = -1.86421698e-006$   
 $f0 = 2600.237$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	2600.237	0.9998	-0.00016
4.4999	2814.700	4.5002	0.00028
15.0001	3533.544	15.0000	-0.00008
18.4998	3799.584	18.4995	-0.00029
24.0000	4245.942	24.0002	0.00022
28.9999	4682.643	29.0001	0.00022
32.5000	5006.484	32.4998	-0.00019

$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 * T_{90}$  (-2 to 35  $^\circ\text{C}$ )

Residual = instrument temperature - bath temperature

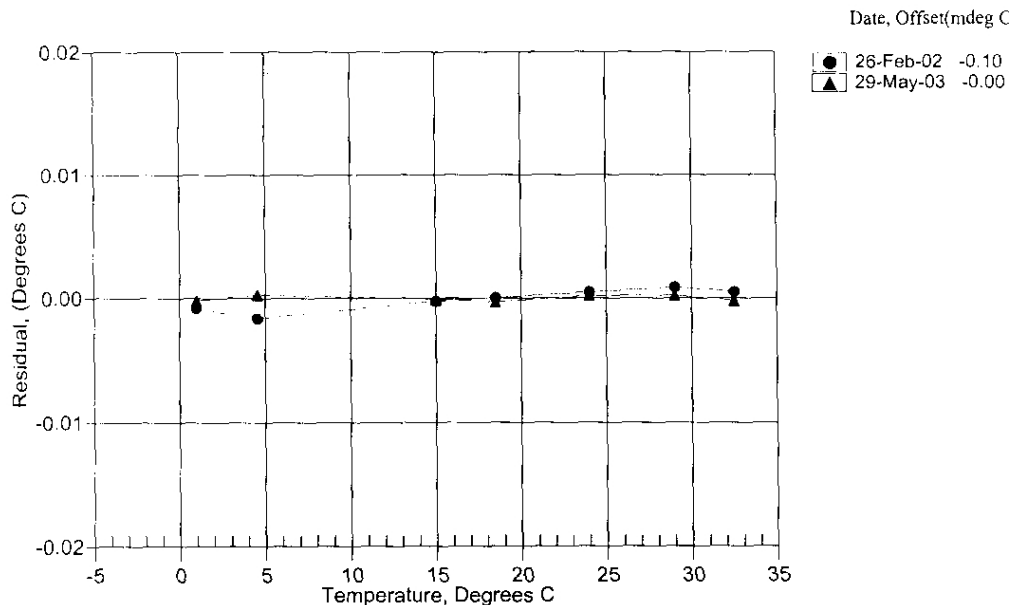

# SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington 98005 USA  
 Phone: (425) 643 - 9866 Fax: (425) 643 - 9954 Internet: seabird@seabird.com

SENSOR SERIAL NUMBER = 857  
 CALIBRATION DATE: 11-Feb-03

TEMPERATURE CALIBRATION DATA  
 ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.24049398e-03$   
 $h = 5.98239597e-04$   
 $i = 3.89001102e-06$   
 $j = -1.91364373e-06$   
 $T_0 = 1000.000$

## IPTS-68 COEFFICIENTS

$a = 3.64763895e-03$   
 $b = 5.84844252e-04$   
 $c = 9.65980297e-06$   
 $d = -1.91318848e-06$   
 $T_0 = 2720.216$


BATH TEMP (ITS-90 °C)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90 °C)	RESIDUAL (ITS-90 °C)
1.0000	2720.216	0.9997	-0.00030
4.4999	2943.126	4.5005	0.00055
15.0000	3689.274	14.9995	-0.00049
18.5001	3965.221	18.5001	-0.00004
24.0001	4427.700	24.0003	0.00023
29.0001	4879.863	29.0004	0.00033
32.5000	5214.905	32.4997	-0.00028

Temperature ITS-90 =  $1/[g + h[\ln(T_0/T)] + i[\ln^2(T_0/T)] + j[\ln^3(T_0/T)]] - 273.15$  (°C)

Temperature IPTS-68 =  $1/[a + b[\ln(T_0/T)] + c[\ln^2(T_0/T)] + d[\ln^3(T_0/T)]] - 273.15$  (°C)

Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 * T_{90}$  (-2 to 35 °C).

Residual = instrument temperature - bath temperature

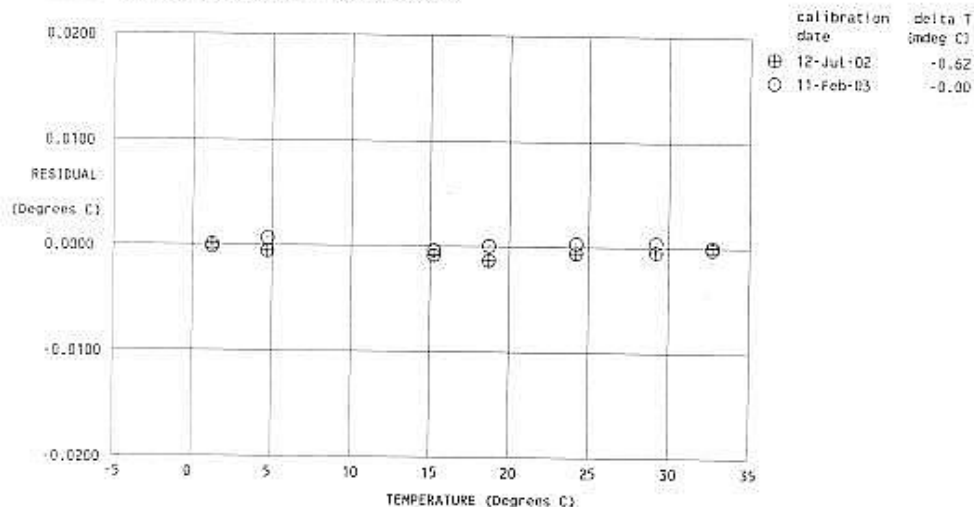

**Underway Remote Temperature Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington 98005 USA  
 Phone: (425) 643 - 9866 Fax: (425) 643 - 9954 Internet: seabird@seabird.com

SENSOR SERIAL NUMBER = 2593  
 CALIBRATION DATE: 06-Feb-03s

TEMPERATURE CALIBRATION DATA  
 ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.27986177e-03$   
 $h = 6.19586021e-04$   
 $i = 2.06496791e-05$   
 $j = 1.61096809e-06$   
 $f_0 = 1000.000$

## IPTS-68 COEFFICIENTS

$a = 3.68121114e-03$   
 $b = 5.83363745e-04$   
 $c = 1.58585118e-05$   
 $d = 1.61237533e-06$   
 $f_0 = 2709.478$


BATH TEMP (ITS-90 °C)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90 °C)	RESIDUAL (ITS-90 °C)
-1.4999	2709.478	-1.4999	-0.00001
1.0001	2870.267	1.0001	0.00003
4.5001	3106.997	4.5001	0.00001
8.0001	3357.687	8.0000	-0.00006
11.5001	3622.778	11.5001	-0.00003
15.0001	3902.688	15.0002	0.00005
18.5001	4197.822	18.5002	0.00007
22.0002	4508.589	22.0002	-0.00004
25.5001	4835.381	25.5001	-0.00000
29.0002	5178.600	29.0001	-0.00007
32.5001	5538.610	32.5001	0.00005

Temperature ITS-90 =  $1/[g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]] - 273.15$  (°C)

Temperature IPTS-68 =  $1/[a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]] - 273.15$  (°C)

Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 * T_{90}$  (-2 to 35 °C).

Residual = instrument temperature - bath temperature

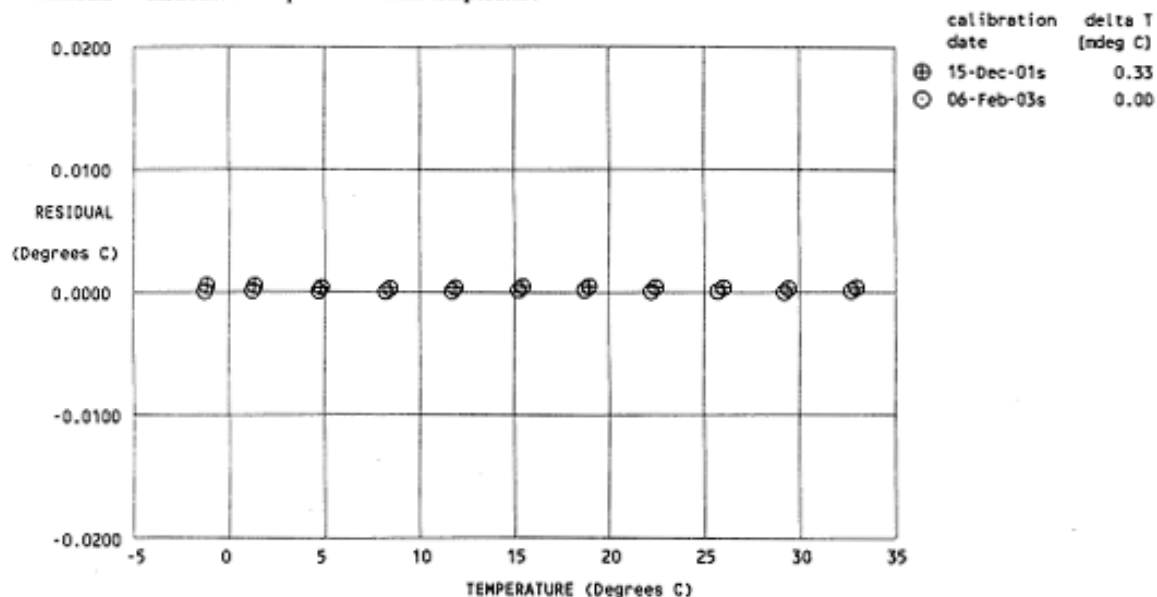

**Underway Transmissometer**

PO Box 518  
620 Applegate St.  
Philomath OR 97370



(541) 929-5650  
Fax (541) 929-5277  
<http://www.wetlabs.com>

**C-Star Calibration Sheet**

**Date:** 02/24/03  
**Customer:** National Science Foundation  
**Serial Number:** CST-422PR  
**Job Number:** 0012016  
**Work Order:** 005

$V_d = V_{\text{dark}}$  0.058  
 $V_{\text{air}} = V_{\text{out in air}}$  4.884  
 $V_{\text{ref}} = V_{\text{out in water}}$  4.772  
Calibration temperature of water 19.6  
Ambient temperature 21.8

$$\% \text{ Transmission} = (V_{\text{sig}} - V_d) / (V_{\text{ref}} - V_d)$$

$$Tr = e^{-cx}$$

To solve for the attenuation coefficient  $c$  in units of  $\text{m}^{-1}$  use the following equation.

$$c = -1/x (\ln(V_{\text{sig}} - V_d) / (V_{\text{ref}} - V_d))$$

For further information on these calculations please see C-Star User's Guide, Section 2.

**Temperature Error: 0.02% F.S./°C**

**NOTES**

- ( $V_d$ )—analog output of the instrument with the beam blocked. This is an instrumental offset.
- ( $V_{\text{air}}$ )—analog output voltage of the instrument with a cleared beam path.
- ( $V_{\text{ref}}$ )—analog output voltage of the instrument with clean  $\text{H}_2\text{O}$  in the path.
- (**Calibration Temperature of water**)—temperature of the clean water used to obtain  $V_{\text{ref}}$ .
- (**Ambient Temperature**)—temperature of the instrument during the calibration procedures.
- ( $V_{\text{sig}}$ )—measured signal voltage of the C-Star.

**Gravity Tie Meter****Gravity Tie Spreadsheet**

The fields outlined in **BOLD** MUST BE FILLED IN for this spreadsheet to operate properly.  
The automatically calculated values show up in the shaded fields.

Date: 12/15/2003  
 Location: Lyttelton/Christchurch, New Zealand  
 Station: Ranger's Hut, Botanical Gardens  
 Latitude: 43 31.77 S  
 Longitude: 172 37.18 E  
 Elevation: 6.7 meters  
 Gravity: 980494.29

## Reference Code Numbers:

ADIC 0217-0  
 IGC 48732A  
 DSIR P11  
 GW 79  
 NHO 16

	Value	Time (GMT)
Ship's meter before gravity tie (Digital Gravity)	8156.2	19:22
Ship's meter after gravity tie (Digital Gravity)	8156.2	23:05
Average:	8156.2	
Ship Gravimeter's Calibration Constant	1.0046	
Corrected ship's meter (Digital Gravity)	8193.7	

	Value	Time (GMT)
Ship's meter before gravity tie (serial, RVDAS)	8193.7	19:33
Ship's meter after gravity tie (serial, RVDAS)	8193.8	23:15
Average (for comparison check only)	8193.8	

Portable Gravimeter Correction Divisor 1.007937

Station	Value	Time (GMT)	Temp	Date	OBS mgal, averaged
Pier measurement 1	4119.53	19:49	53.5	December 15, 2003	
Pier measurement 2	4119.43	19:52	53.5	December 15, 2003	4087.09
Pier measurement 3	4119.62	19:54	53.5	December 15, 2003	
Average	4119.53				
Station measurement 1	4088.11	21:11	53.5	December 15, 2003	
Station measurement 2	4088.12	21:14	53.5	December 15, 2003	4055.94
Station measurement 3	4088.16	00:00	53.5	December 15, 2003	
Average	4088.13				
Pier measurement 4	4119.68	23:05	53.5	December 15, 2003	
Pier measurement 5	4119.64	23:07	53.5	December 15, 2003	4087.22
Pier measurement 6	4119.69	23:11	53.5	December 15, 2003	
Average	4119.65				

Gravity offset from last tie 972337.78  
 Drift since last tie -5.52

**OBS Differences**

Station to Pier (1, 2, & 3 averaged) 31.15  
 Station to Pier (4, 5, & 6 averaged) 31.29  
 Averaged Differences 31.22  
 Gravity at pier 980525.51  
 Elevation of pier above gravimeter, meters -1.8  
 Earth differential gravity, mgal/meter 0.3  
 Gravity at ship's gravimeter 980524.98  
 Gravity Offset 972331.26

**Comments**

Tie completed by W. Gallagher and F. Trujillo. Rebuilt gyros were installed by J. Otten during the port period just prior to this tie.