


NBP0603 RVDAS Data Report

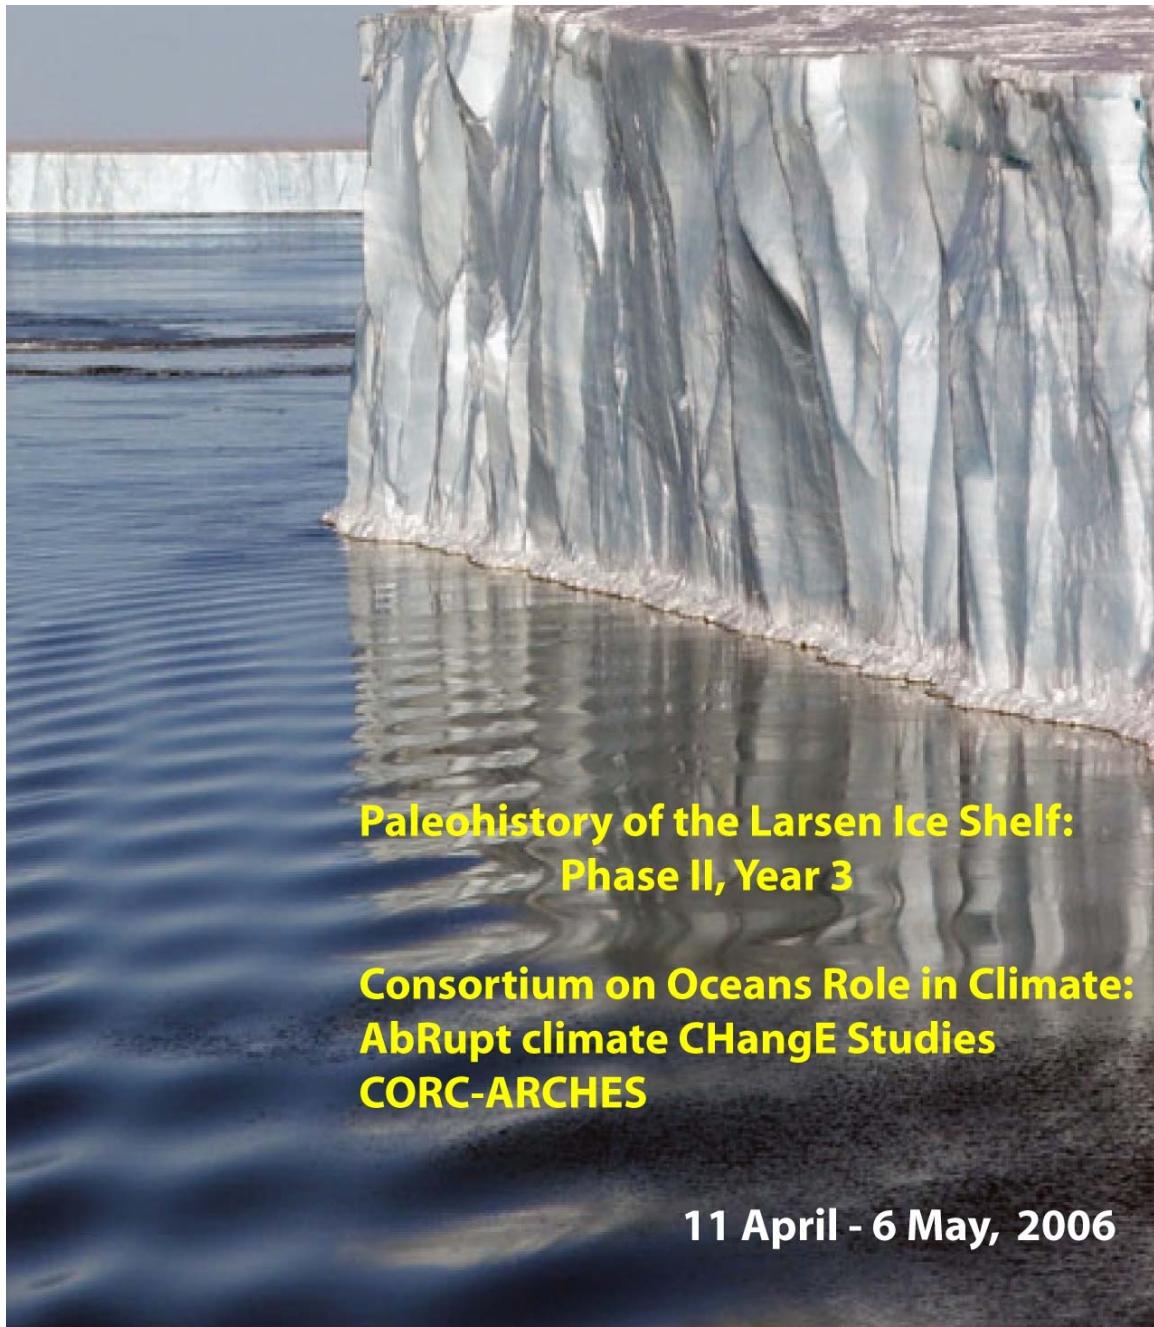

Prepared by: Paul G. Huckins and Isaiah Norton
Raytheon Polar Services Company
US Antarctic Program

Table of Contents

INTRODUCTION.....	1
ARCHIVE COMMANDS	1
DISTRIBUTION CONTENTS AT A GLANCE	2
DISTRIBUTION CONTENTS	3
CRUISE INFORMATION.....	3
<i>Cruise Track</i>	3
<i>Satellite Images</i>	3
<i>Science Reports</i>	3
NBP DATA PRODUCTS.....	3
<i>JGOFS</i>	3
<i>MGD77</i>	4
SCIENCE OF OPPORTUNITY.....	5
<i>ADCP</i>	5
<i>pCO₂</i>	6
CRUISE SCIENCE	6
XBT	6
RVDAS	6
<i>Sensors and Instruments</i>	6
Underway Sensors	7
Meteorology and Radiometry	7
Geophysics	7
Oceanography.....	7
Navigational Instruments	7
<i>Raw Data</i>	8
Underway Data	9
Sound Velocity Probe (svp1).....	9
Meteorology (met1).....	9
Gravimeter (grv1).....	10
Bathy 2000 (bat1).....	11
Knudsen (knud).....	12
Simrad EM120 (mbdp).....	12
Simrad EK500 (sim1).....	13
Thermosalinograph (tsg1)	13
Fluorometer (flr1).....	13
pCO ₂	13
Navigational Data	14
Seapath GPS (seap)	14
Trimble (P-Code) GPS (PCOD)	17
Gyro Compass (gyr1)	18
ADCP Course (adcp).....	18
Sound Velocity Probe (svp1).....	18
<i>Processed Data</i>	19
pCO ₂ -merged	19
tsgfl.....	19
CALCULATIONS.....	20
TSG	20
PAR	21
PIR.....	21
PSP	21
ACQUISITION PROBLEMS AND EVENTS.....	22
APPENDIX: SENSORS AND CALIBRATIONS.....	23
NBP0603 SENSORS:.....	23

<i>Shipboard Sensors</i>	23
<i>NBP0601 CTD Sensors</i>	24
CALIBRATIONS	24
GRAVITY TIE.....	25
METEOROLOGY SYSTEM	26
<i>Anemometer (Port)</i>	26
<i>Anemometer (Starboard)</i>	27
<i>PIR</i>	28
<i>PSP</i>	29
<i>GUV</i>	30
<i>PUV</i>	31
<i>PAR</i>	32
TSG CALIBRATION FILES.....	33
<i>Underway Conductivity</i>	33
<i>Underway Temperature Sensor</i>	34
<i>Underway Remote Temperature Sensor</i>	35
<i>Underway Transmissometer</i>	36
CTD SENSORS.....	37
<i>CTD Fish Pressure Sensor</i>	37
<i>CTD Temperature (Primary)</i>	38
<i>CTD Temperature (Secondary)</i>	39
<i>CTD Conductivity (Primary)</i>	40
<i>CTD Conductivity (Secondary)</i>	41
<i>CTD Fluorometer</i>	42
<i>CTD Transmissometer</i>	43
<i>CTD Dissolved Oxygen Sensor</i>	44

Introduction

The NBP data acquisition systems continuously logs data from the instruments used during the cruise. This document describes:

- The structure and organization of the data on the distribution media
- The format and contents of the data strings
- Formulas for calculating values
- Information about the specific instruments in use during the cruise
- A log of acquisition problems and events during the cruise that may affect the data
- Scanned calibration sheets for the instruments in use during the cruise.

The data is distributed on a DVD-R written in ISO9660 level-1 format. It is readable by virtually every computing platform.

All data has been packaged in Unix tar archive files. Most files inside the tar archive have been compressed to reduce size. Compressed files are identified by the extension “gz”. Tools are available on all platforms for uncompressing and de-archiving these files:

On Macintosh, use Stuffit Expander with DropStuff or the command line utilities.

On Windows, use WinZip or the freeware program 7zip (installer is located in /other/7zip.exe).

tar, gzip, and gunzip are standard tools on all Unix and Unix-like systems.

MultiBeam and BathyW data are distributed separately.

IMPORTANT: Read the last section, “Acquisition Problems and Events,” for important information that may affect the processing of this data.

Archive Commands

All archives were created using the command:

```
tar [z]cvf archive_name files_to_archive
```

With [z] being used to create “.tgz” archives.

To create a list of the files in the archive, use the Unix command:

```
tar [z]tvf archive_name > contents.list
```

where contents.list is the name of the file to create

To extract the files from the archive:

```
tar [z]xvf archive_name file(s)_to_extract
```

Distribution Contents at a Glance

Volume 1

NBP0603.gmt	rvdas/nav/	
NBP0603.mgd		0603adcpt.tar
0603BE.gmt		0603gyr1.tar
NBP0603.trk		0603PCOD.tar
0603data.doc		0603seap.tar
0603data.pdf		0603sp2a.tar
trkmaps.tar		
INSTCOEF.TXT	rvdas/uw/	
adcpt/		0603bat1.tar
	0603mat.tar	0603eng1.tar
images/		0603flr1.tar
	isobars.tar	0603grv1.tar
	ice.tar	0603knud.tar
	wx.tar	0603mbdp.tar
ocean/		0603met1.tar
	0603ctd.tar	0603oyo1.tar
	0603xbt.tar	0603pco2.tar
process/		0603pguv.tar
	0603JGOF.tar	0603svp1.tar
	0603MGD.tar	0603syn1.tar
	0603PCO2.tar	0603tsg1.tar
	0603PROC.tar	
	0603QC.tar	
	scirep/	
		<i>Weekly cruise reports in rich-text and PDF format.</i>
	other/	
		7zip.exe

Volume 2

Seismic/	Seg-Y files from Triton Elics system
Bathy2kw/	Seg-Y files from the Bathy2KW system

Distribution Contents

Cruise Information

NBP0603 was a marine geology cruise running from Punta Arenas, Chile 11 April 2006 to Punta Arenas, Chile 6 May 2006.

Cruise Track

The distribution DVD includes a GMT cruise track file (NBP0603.trk). It contains the longitude and latitude at one-minute intervals extracted from the NBP0603.gmt file.

A plot of the cruise track is available in postscript, pdf, and jpeg formats, in the files: 0603trk.jpg, 0603trk.pdf, and 0603trk.ps.

Satellite Images

Satellite, weather, and isobar images processed during this cruise can be found in the directory /images in three tar files: ice.tar, isobar.tar, and wx.tar (weather).

Science Reports

Weekly cruise science reports are located in the directory /scirep.

NBP Data Products

Two primary datasets are created on each cruise: JGOFS and MGD77.

The data processing scripts used to produce JGOFS and MGD77 data sets create a number of intermediate files. These files are included on the data distribution media in a file called 0603proc. They are included to make re-processing easier in the event of an error, but no extensive detail of the formats is included in this document. For information, please contact itvessel@usap.gov.

JGOFS

The JGOFS data set may be found on the distribution media in the file /process/0603JGOF.tar. The archive contains one file produced for each day named jgDDD.dat.gz, where DDD is the year-day the data was acquired. The ".gz" extension indicates that the individual files are compressed before archiving. Each daily file consists of 22 columnar fields in text format as described in the table below. The JGOFS data set is created from calibrated data decimated at one-minute intervals. Several fields are derived measurements from more than a single raw input. For example, Course Made Good (CMG) and Speed Over Ground (SOG) are calculated from gyro and GPS inputs. Daily plots during the cruise are produced from the JGOFS data set. Note: Null, unused, or unknown fields are indicated as "NAN" as 9999 in the JGOFS data.

Field	Data	Units
01	GMT date	dd/mm/yy
02	GMT time	hh:mm:ss
03	NGL latitude (negative is South)	tt.tttt
04	NGL longitude (negative is West)	ggg.gggg
05	Speed over ground	Knots
06	GPS HDOP	-
07	Gyro Heading	Degrees (azimuth)
08	Course made good	Degrees (azimuth)

Field	Data	Units
09	Mast PAR	μ Einstens/meter ² sec
10	Sea surface temperature	°C
11	Sea surface conductivity	siemens/meter
12	Sea surface salinity	PSU
13	Sea depth (uncorrected, calc. sw sound vel. 1500 m/s)	meters
14	True wind speed (max speed windbird)	meters/sec
15	True wind direction (max speed windbird)	degrees (azimuth)
16	Ambient air temperature	°C
17	Relative humidity	%
18	Barometric pressure	mBars
19	Sea surface fluorometry	volts (0-5 FSO)
20	Not used	-
21	PSP	W/m ²
22	PIR	W/m ²

MGD77

The MGD77 data set is contained in a single file for the entire cruise. It can be found in the top level of the distribution data structure as NBP0603.mgd. The file NBP0603.gmt is created from the MGD77 dataset using the "mgd77togmt" utility. NBP0603.gmt can be used with the GMT plotting package.

The data used to produce the NBP0603.mgd file can be found at the root of the distribution media and in the file /process/0603proc.tar. The data files in the archive contain a day's data and follow the naming convention Dddd.fnl.gz, where ddd is the year-day. These files follow a space-delimited columnar format that may be more accessible for some purposes. They contain data at one-second intervals rather than one minute and are individually "gzipped" to save space. Below is a detailed description of the MGD77 data set format.

All decimal points are implied. Leading zeros and blanks are equivalent. Unknown or unused fields are filled with 9's. All "corrections", such as time zone, diurnal magnetics, and EOTVOS, are understood to be added.

Col	Len	Type	Contents	Description, Possible Values, Notes
1	1	Int	Data record type	Set to "5" for data record
2-9	8	Char	Survey identifier	
10-12	3	int	Time zone correction	Corrects time (in characters 13-27) to GMT when added; 0 = GMT
13-16	4	int	Year	4 digit year
17-18	2	int	Month	2 digit month
19-20	2	int	Day	2 digit day
21-22	2	int	Hour	2 digit hour
23-27	5	real	Minutes x 1000	
28-35	8	real	Latitude x 100000	+ = North - = South. (-9000000 to 9000000)
36-44	9	real	Longitude x 100000	+ = East - = West. (-18000000 to 18000000)
45	1	int	Position type code	1=Observed fix 3=Interpolated 9=Unspecified
46-51	6	real	Bathymetry, 2-way travel time	In 10,000th of seconds. Corrected for transducer depth and other such corrections
52-57	6	real	Bathymetry, corrected depth	In tenths of meters.

Col	Len	Type	Contents	Description, Possible Values, Notes
58-59	2	int	Bathymetric correction code	This code details the procedure used for determining the sound velocity correction to depth
60	1	int	Bathymetric type code	1 = Observed 3 = Interpolated (Header Seq. 12) 9 = Unspecified
61-66	6	real	Magnetics total field, 1 ST sensor	In tenths of nanoteslas (gammas)
67-72	6	real	Magnetics total field, 2 ND sensor	In tenths of nanoteslas (gammas), for trailing sensor
73-78	6	real	Magnetics residual field	In tenths of nanoteslas (gammas). The reference field used is in Header Seq. 13
79	1	int	Sensor for residual field	1 = 1 st or leading sensor 2 = 2 nd or trailing sensor 9 = Unspecified
80-84	5	real	Magnetics diurnal correction	In tenths of nanoteslas (gammas). (In nanoteslas) if 9-filled (i.e., set to "+9999"), total and residual fields are assumed to be uncorrected; if used, total and residuals are assumed to have been already corrected.
85-90	6	F6.0	Depth or altitude of magnetics sensor	(In meters) + = Below sea level 3 = Above sea level
91-97	7	real	Observed gravity	In 10 th of mgals. Corrected for Eotvos, drift, tares
98-103	6	real	EOTVOS correction	In 10 th of mgals. E = 7.5 V cos phi sin alpha + 0.0042 V*V
104-108	5	real	Free-air anomaly	In 10 th of mgals G = observed G = theoretical
109-113	5	char	Seismic line number	Cross-reference for seismic data
114-119	6	char	Seismic shot-point number	
120	1	int	Quality code for navigation	5=Suspected, by the originating institution 6=Suspected, by the data center 9=No identifiable problem found

Science of Opportunity

ADCP

The ADCP system measures currents in a depth range up to 1200 m (OS38 in deep profiling mode). In bad weather, ice, or unfavorable sea state the range is reduced, and sometimes no valid measurements are made. ADCP data collection is the OPP-funded project of Eric Firing (University of Hawaii) and Teri Chereskin (Scripps Institution of Oceanography). Data is collected on both the LMG and the NBP for the benefit of scientists on each cruise, and for the long-term goal of building a profile of current structure in the Southern Ocean.

Matlab ".mat" files containing current contour and vector data have been placed in the file /adcp/0603MAT.tar. Please note that these files must be considered preliminary only. Data are not a "final product" until post-processing has been performed by the principal investigators. For more information on data format, post-processing, and for data download, please visit: <http://currents.soest.hawaii.edu>

A data feed is sent from the ADCP system to RVDAS whenever a reference layer is acquired. This feed contains east and north vectors for ship's speed, relative to the reference layer, and ship's heading. This data is saved in files located in `0603adcp.tar` in the directory `/rvdas/nav`.

pCO₂

The NBP carries a pCO₂ measurement system from Lamont-Doherty Earth Observatory (LDEO). pCO₂ data is recorded by RVDAS and transmitted to LDEO at the end of each cruise. pCO₂ data is archived in the file `0603pc02.tar` in the `/process` directory, which contains the pCO₂ instrument's data merged with GPS, meteorological and other oceanographic measurements. For more information contact Colm Sweeney (`csweeney@ldeo.columbia.edu`).

Cruise Science

XBT

During the cruise, eXpendable BathyThermographs were used to obtain water column temperature profiles. XBT profiles allow corrections to the sound velocity profile for the multi-beam system. The data files from these launches are included as `603xbt.tar` in the `/ocean` directory.

RVDAS

The Research Vessel Data Acquisition System (RVDAS) was developed at Lamont-Doherty Earth Observatory of Columbia University and has been in use on its research ship for many years. It has been extensively adapted for use on the USAP research vessels.

Daily data processing of the RVDAS data is performed to calibrate and convert values into useable units and as a check of the proper operation of the DAS. Both raw and processed data sets from RVDAS are included in this data distribution. Quality-control plots for most instruments are created daily, and may be found in postscript format in the file `/process/0603QC.tar`. The tables below provide detailed information on the sensors and data. Be sure to read the "Significant Acquisition Events" section for important information about data acquisition during this cruise.

Sensors and Instruments

RVDAS data is divided into two general categories, *underway and navigation*. Raw data will be found on the distribution media as subdirectories under the top level `rvdas` directory: `/rvdas/uw`, and `/rvdas/nav`. Each instrument or sensor produces a data file named with its channel ID. Each data file is g-zipped to save space on the distribution media. Not all data types are collected every day or on every cruise.

The naming convention for data files produced by the sensors and instruments is

NBP[CruiseID][ChannelID].dDDD

Example: NBP0107met1.d317

- The CruiseID is the numeric name of the cruise, in this case, NBP603.
- The ChannelID is a 4-character code representing the system being logged. For example the meteorology designation is "met1".
- DDD is the day of year the data was collected

Underway Sensors

Meteorology and Radiometry

Measurement	Channel ID	Collect. Status	Rate	Instrument
Air Temperature	met1	Continuous	1 sec	R. M. Young 41372LC
Relative Humidity	met1	Continuous	1 sec	
Wind Speed/Direction	met1	Continuous	1 sec	R.M. Young 5106
Barometer	met1	Continuous	1 sec	R.M. Young 61201
PIR (LW radiation)	met1	Continuous	1 sec	Eppley PIR
PSP (SW radiation)	met1	Continuous	1 sec	Eppley PSP
PAR	met1	Continuous	1 sec	BSI QSR-240
GUV	guv	Continuous	2 sec	BSI PUV-2511
PUV	puv	Continuous		BSI PUG-2500

Geophysics

Measurement	Channel ID	Collect. Status	Rate	Instrument
Gravimeter	grv1	Continuous	10 sec*	LaCoste & Romberg
Magnetometer	mag1	Not collected	15 sec	EG&G G-866
Bathymetry	bat1	Per direction	Varies	ODEC Bathy 2000
Bathymetry	knu1	Per direction	Varies	Knudsen 320B/R
Bathymetry	sim1	Not collected	Varies	Simrad EK500 Sonar

*Data is output every second but only changes every 10 seconds.

Oceanography

Measurement	Channel ID	Collect. Status	Rate	Instrument
Conductivity	tsg1	Continuous	6 sec	SeaBird SBE-21
Salinity	tsgfl	Continuous	6 sec	Calc. from pri. temp
Sea Surface Temp	tsg1	Continuous	6 sec	SeaBird 3-01/S
Fluorometry	flr1	Continuous	1 sec	Turner 10-AU-005
Fluorometry	flr1 & tsg1	Continuous	6 sec	
Transmissometry	tsg1	Continuous	6 sec	WET Lab C-Star
pCO ₂	pco2	Continuous	70 sec	(LDEO)
ADCP	adcp	Continuous	varies	RD Instruments

Navigational Instruments

Measurement	Channel ID	Collect. Status	Rate	Instrument
Trimble GPS	PCOD	Continuous	1 sec	Trimble 20636-00SM
Gyro	gyr1	Continuous	0.2 sec	Yokogawa Gyro
SeaPath	seap	Continuous	1 sec	SeaPath 200

Raw Data

Data is received from the instrument system via RS-232 serial connections. A time tag is added by RVDAS at the beginning of each line of data in the form,

yy+dd:hh:mm:ss.sss [data stream from instrument]

where

yy = two-digit year
ddd = day of year
hh = 2 digit hour of the day
mm = 2 digit minute
ss.sss = seconds

All times are reported in UTC.

The delimiters that separate fields in the raw data files are often spaces and commas but can be other characters such as : = @. Occasionally no delimiter is present. Care should be taken when reprocessing the data that the field's separations are clearly understood.

In the sections below a sample data string is shown, followed by a table that lists the data contained in the string.

Underway Data

Sound Velocity Probe (svp1)

00+348:01:59:52.128 1539.40

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

Meteorology (met1)

01+322:00:03:27.306 04.5 292 010 05.7 294 010 0959.6 000.2 093.1

-000.1537 0001.0886 0012.8248

Field	Data	Units
1	RVDAS time tag	
2	Port anemometer speed (relative)	m/s
3	Port anemometer direction (relative)	deg
4	Port anemometer standard deviation	deg
5	Starboard anemometer speed (relative)	m/s
6	Starboard anemometer direction (relative)	deg
7	Starboard anemometer standard deviation	deg
8	Barometer	mBar
9	Air temperature	°C
10	Relative humidity	%
11	PSP (short wave radiation)*	mV
12	PIR (long wave radiation)*	mV
13	PAR (photo synthetically available radiation)*	mV

*See page 20 for calculations.

Gravimeter (grv1)

There are two sets of fields output by the gravity meter. The data record is output once per second, and identified by "\$DAT" in the id field. A summary of sensor environmental data is output every ten seconds, identified by "%ENV" in the id field.

Data record (\$DAT):

```
05+194:00:00:27.995 $DAT,2005/ 7/13, 0: 7: 7.36,194, 9050.37, 9050.06, 5410.86, -0.00, -
0.01, -0.02, 0.00, 0.00, 0.70, 0.19, -0.12, -0.25, 0.00, -69.45711315, -54.32181487,
0.000, 285.200,
```

Field	Data	Conversion	Units
1	RVDAS time tag		
2	Text string (id field)	\$DAT for data record	
3	Date	YYYY/MM/DD	
4	Time	HH:MM:SS.SS	
5	Day of Year	DDD	
6	Gravity count	mgal = count x 1.0046 + offset	count
7	Spring Tension		CU
8	Beam Position	Volts x 750,000	
9	VCC		
10	AL		
11	AX		
12	VE		
13	AX2		
14	XACC2		
15	LACC2		
16	CROSS ACCEL		GAL
17	LONG ACCEL		GAL
18	EOTVOS CORR		MGAL
19	LONGITUDE		Degrees
20	LATITUDE		Degrees
21	HEADING		Degrees
22	VELOCITY		Knots

Environmental record (\$ENV)

```
05+183:19:13:10.945 %ENV,2005/ 7/ 2,19:19:52.16,183,S-036/V1.5, 3.34,
47.19, 20.34,1.111840E-1,-0.57700,-0.10591, 0.40180, 2.55260, 0.43000,
1, 300
```

Field	Data	Conversion	Units
1	RVDAS time tag		
2	Text string (id field)	\$ENV for environmental record	
3	Date	YYYY/MM/DD	
4	Time	HH:MM:SS.SS	
5	Day of Year	DDD	
6	Meter ID		
7	Meter Pressure		inch-Hg
8	Meter temp		°C
9	Ambient temp		°C
10	K-Factor		
11	VCC Coeff		

Field	Data	Conversion	Units
12	AL Coeff		
13	AX Coeff		
14	VE Coeff		
15	AX2 Coeff		
16	Serial Filter Length		Seconds
17	QC Filter Length		Seconds

Bathy 2000 (bat1)

00+019:23:59:53.901 ;I04485.3ME -23.0, I00000.0,-99.9,0000@01/11/00,
23:59:52.08 PW2 PF1 SF1 PL3 MO4 SB3 PO0 TX1 TR: GM5 1500 06.7 -72.1

Field	Data	Format / Possible Values	Units
1	RVDAS time tag		
2	Flagged low frequency chn. depth w/ units	;FDDDDDD.Dun where F = flag (V for valid, I for invalid), D=depth, un = units	meters
3	Low Frequency echo strength	EEE.EE	dB
4	Flagged high freq. chn. depth	not used	
5	High frequency echo strength	not used	
6	Signed heave data	SHHHH	cm
7	Date	mm/dd/yy	
8	Time	hh:mm:ss	
9	Transmit pulse window type	PW1=Rectangular PW2=Hamming PW3=Cosine PW4=Blackman	
10	Primary transmit frequency	PF1=3.5 kHz PF2=12.0 kHz	kHz
11	Parametric mode secondary frequency	SF1=3.5 kHz SF2=12.0 kHz	kHz
12	Pulse length	PL1=200usec PL2=500usec PL3=1msec PL4=2msec PL5=5msec PL6=10msec PL7=25msec If transmit mode is FM: PL1=25msec PL2=50msec PL3=100msec	
13	Operating mode	MO1=CW parametric MO2=CW MO3=FM parametric MO4=FM	
14	Frequency sweep bandwidth	SB1=1 kHz SB2=2 kHz SB3=5 kHz	kHz
15	Power level	PO1 = 0dB PO2 = -6dB PO3 = -12dB PO4 = -18dB PO5 = -24dB PO6 = -30dB PO6 = -30 dB	

Field	Data	Format / Possible Values	Units
		PO7 = -36dB PO8 = -42dB	
16	Transmit mode	TX1=single ping active TX2=pinger listen TX3=multipinging TR TX4=multipinging TR TX5=multipinging TTRR TX6=multipinging TTTTRRRR TX7=multipinging TTTTTRRRRR	
17	Transmit Rate	TR3 = 4Hz TR4 = 2Hz TR5 = 1Hz TR6 = .5Hz TR7 = .33Hz TR8 = .25Hz TR9 = .20Hz TR; = .10Hz TR; = .05Hz	Hz
18	System gain mode	GM0=hydrographic AGC GM1 to GM9=hydrographic +3db to + 27db manual. GMA to GMD=hydrographic + 30db through + 60db manual GME to GMK=sub-bottom 1 through sub-bottom 7	
19	Speed of sound		m/sec
20	Depth of sonar window below sea-level		meters
21	Background noise level in fixed point reference		dB/V

Knudsen (knud)

99+099:00:18:19.775 HF,305.2,LF,304.3

Field	Data	Units
1	RVDAS time tag	
2	HF = High frequency flag (12 kHz)	
3	High frequency depth	meters
4	LF = Low frequency flag (3.5 kHz)	
5	Low frequency depth	meters

Simrad EM120 (mbdp)

Field	Data	Units
1	LDTDS	
2	\$EMDPT	
3	Depth (corrected)	Meters

Simrad EK500 (sim1)

00+005:00:00:52.388 D1,23583509,1479.6, 17, 1, 0

Field	Data	Units
1	RVDAS time tag	
2	Header	
3	Time tag	hhmmss.sss
4	Depth	m
5	Bottom surface backscattering strength	dBar
6	Transducer number (1 = 38 kHz)	
7		

Thermosalinograph (tsg1)

00+019:23:59:46.976 15A16CFC163F8C2C100

Field	Data	Units
1	RVDAS time tag	
2	Seabird hex string (see page 20 for conversion to real units)	

Fluorometer (flr1)

00+019:23:59:58.061 0 0818 :: 1/19/00 17:23:17 = 0.983 (RAW) 1.2 (C)

Field	Data	Units
1	RVDAS time tag	
2	Marker 0 to 8	
3	4-digit index	
4	Date	mm/dd/yy
5	Time	hh:mm:ss
6	Signal	
7	Signal units of measurement	
8	Cell temperature (if temperature compensation package is installed)	
9	Temperature units (if temperature compensation package is installed)	

pCO200+021:23:59:43.190 2006114.02630 1960.80 20.64 1003.5 346.81 -1.63
341.7 52.49 0 13 Equil

Field	Data	Units
1	RVDAS time tag	
2	pCO ₂ time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temp (C)	°C
5	Barometric pressure (mbar)	MBar
6	CO ₂ conc. (ppm)	ppm
7	Equilibrator Temp (C)	°C
8	pCO ₂ pressure (uatm)	microAtm
9	Flow rate (cc/min)	ml / min
10	Valve Position (integer, note position 9 does not write, defaults to 1)	1 or 2 digits
11	Sample Code number (integer)	1 or 2 digits
12	Flow source (Equil = pCO ₂ measurement)	text

Navigational Data

Seapath GPS (seap)

The Seapath GPS outputs the following data strings, four in NMEA format and two in proprietary PSXN format:

- GPZDA
- GPGGA
- GPVTG
- GPHDT
- PSXN, 20
- PSXN, 22
- PSXN, 23

GPZDA

02+253:00:00:00.772 \$GPZDA,235947.70,09,09,2002,,*7F

Field	Data	Units
1	RVDAS time tag	
2	\$GPZDA	
3	time	hhmmss.ss
4	Day	dd
5	Month	mm
6	Year	yyyy
7	(empty field)	
8	Checksum	

GPGGA

02+253:00:00:00.938

GPGGA,235947.70,6629.239059,S,06827.668899,W,1,07,1.0,11.81,M,,M,,*6F

Field	Data	Units
1	RVDAS time tag	
2	\$GPGGA	
3	time	hhmmss.ss
4	Latitude	ddmm.mmmmmmm
5	N or S for north or south latitude	
6	Longitude	ddmm.mmmmmmm
7	E or W for east or west longitude	
8	GPS quality indicator, 0=invalid, 1=GPS SPS, 2=DGPS, 3=PPS, 4=RTK, 5=float RTK, 6=dead reckoning	
9	number of satellites in use (00-99)	
10	HDOP	x.x
9	height above ellipsoid in meters	m.mm
11	M	
12	(empty field)	
13	M	
14	age of DGPS corrections in seconds	s.s
15	DGPS reference station ID (0000-1023)	

Field	Data	Units
16	Checksum	

GPVTG

02+253:00:00:00.940 \$INVTG,19.96,T,,M,4.9,N,,K,A*39

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	course over ground, degrees true	d.dd
4	T	
5	,	
6	M	
7	speed over ground in knots	k.k
8	N	
9	,	
10	K	
11	Mode	
12	Checksum	

GPHDT

02+253:00:00:00.941 \$GPHDT,20.62,T*23

Field	Data	Units
1	RVDAS time tag	
2	\$GPHDT	
3	Heading, degrees true	d.dd
4	T	
5	Checksum	

PSXN,20

02+253:00:00:00.942 \$PSXN,20,0.43,0.43*39

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	20	
4	Horizontal position & velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
5	Height & vertical velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
6	Heading quality: 0=normal, 1=reduced performance, 2=invalid data	
7	Roll & pitch quality: 0=normal, 1=reduced performance, 2=invalid data	
8	Checksum	

PSXN,22

02+253:00:00:00.942 \$PSXN,22,0.43,0.43*39

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	22	
4	gyro calibration value since system start-up in degrees	d.dd
5	short term gyro offset in degrees	d.dd
6	Checksum	

PSXN,23

02+253:00:00:02.933 \$PSXN,23,0.47,0.57,20.62,0.03*0C

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	23	
4	roll in degrees, positive with port side up	d.dd
5	pitch in degrees, positive with bow up	d.dd
6	Heading, degrees true	d.dd
7	heave in meters, positive down	m.mm
8	Checksum	

Trimble (P-Code) GPS (PCOD)

The Trimble GPS, which formerly output Precise Position (*P-Code*) strings, but now only outputs Standard Position (*Civilian*) strings, outputs three NMEA standard data strings:

- Position fix (GGA)
- Latitude / longitude (GLL),
- Track and ground speed (VTG)

GGA: GPS Position Fix – Geoid/Ellipsoid

01+319:00:04:11.193 \$GPGGA,000410.312,6227.8068,S,06043.6738,W,1,06,1.0,
031.9,M,-017.4,M,,*49

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGGA	
3	UTC time at position	hhmmss.sss
4	Latitude	ddmm.mmm
5	North (N) or South (S)	
6	Longitude	ddmm.mmm
7	East (E) or West (W)	
8	GPS quality: 0 = Fix not available or invalid 1 = GPS, SPS mode, fix valid 2 = DGPS (differential GPS), SPS mode, fix valid 3 = P-CODE PPS mode, fix valid	
9	Number of GPS satellites used	
10	HDOP (horizontal dilution of precision)	
11	Antenna height	meters
12	M for meters	
13	Geoidal height	meters
14	M for meters	
15	Age of differential GPS data (no data in the sample string)	
16	Differential reference station ID (no data in the sample string)	
17	Checksum (no delimiter before this field)	

GLL: GPS Latitude/Longitude

01+319:00:04:11.272 \$GPGLL,6227.8068,S,06043.6738,W,000410.312,A *32

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGLL	
3	Latitude	degrees
4	North or South	
5	Longitude	degrees
6	East or West	
7	UTC of position	hhmmss.sss
8	Status of data (A = valid)	
9	Checksum	

VTG: GPS Track and Ground Speed

01+319:00:04:11.273 \$GPVTG,138.8,T,126.0,M,000.0,N,000.0,K *49

Field	Data	Units
-------	------	-------

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	Heading	degrees
4	Degrees true (T)	
5	Heading	degrees
6	Degrees magnetic (M)	
7	Ship speed	knots
8	N = knots	
9	Speed	km/hr
10	K = km per hour	
11	Checksum	

Gyro Compass (gyr1)

00+019:23:59:59.952 \$HEHDT 25034,-020 *73

Field	Data	Units
1	RVDAS time tag	
2	\$HEHDT	
3	Heading, Degrees True	degrees
4	Rate of change SYYY S = +/-, YYYY = r.rr	
5	Checksum	

ADCP Course (adcp)

00+019:23:59:59.099 \$PUHAW,UVH,-1.48,-0.51,250.6

Field	Data	Units
1	RVDAS time tag	
2	\$PUHAW	
3	UVH (E-W, N-S, Heading)	
4	Ship Speed relative to reference layer, east vector	knots
5	Ship Speed relative to reference layer, north vector	knots
6	Ship heading	degrees

Sound Velocity Probe (svp1)

00+348:01:59:52.128 1539.40

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

Processed Data

pCO2-merged

00+346:23:58:20.672 2000346.9991 2398.4 1008.4 0.01 45.4 350.3 342.6
 15.77 Equil -43.6826 173.1997 15.51 33.90 0.33 5.28 9.05 1007.57 40.0
 14.87 182.44

Field	Data	Units
1	RVDAS time tag	
2	pCO ₂ time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temp (C)	°C
5	Barometric pressure (mbar)	MBar
6	CO ₂ conc. (ppm)	ppm
7	Equilibrator Temp (C)	°C
8	pCO ₂ pressure (uatm)	microAtm
9	Flow rate (cc/min)	ml / min
10	Valve Position (integer, note position 9 does not write, defaults to 1)	1 or 2 digits
11	Sample Code number (integer)	1 or 2 digits
12	Flow source (Equil = pCO ₂ measurement)	text
13	RVDAS latitude	degrees
14	RVDAS longitude	degrees
15	TSG external temperature	°C
16	TSG salinity (PSU)	PSU
17	TSG fluorometry (mV -0-5)	V
18	RVDAS true wind speed	m/s
19	RVDAS true wind direction	degrees
20	Barometric Pressure	mBars
21	Uncontaminated seawater pump flow rate	l/min
22	Speed over ground (knots)	knots
23	Course made good (deg)	degrees

tsgfl

00+075:00:00:04.467 -01.488 -01.720 02.6783 33.63748 1.002442 0.002442

Field	Data	Units
1	RVDAS time tag	
2	Internal water temperature	°C
3	Sea Surface Temperature	°C
4	Conductivity	µSiemens
5	Salinity	PSU
6	Fluorometry	V
7	Transmissivity	V

Calculations

The file `instcoef.txt` located in the `/` directory contains the calibration factors for shipboard instruments. This was the file used by the RVDAS processing software.

TSG

Raw TSG data is stored as a 20 byte (character) long hex string

Bytes	Data
1-4	Sensor Temperature
5-8	Conductivity
9-14	Remote Temperature
15-17	Fluorometer voltage
18-20	Transmissometer voltage

The coefficients for temperature and conductivity sensors can be found the `rvdascal.txt` file and on the calibrations sheets in the appendix.

Calculating Temperature – ITS-90

```
T = decimal equivalent of bytes 1-4
Temperature Frequency: f = T/19 +2100
Temperature = 1/{g + h[ln(f₀/f)] + i[ln²(f₀/f)] + j[ln³(f₀/f)]} - 273.15 (°C)
```

Calculating Conductivity – ITS-90

```
C = decimal equivalent of bytes 5-8
Conductivity Frequency f = sqrt(C*2100+6250000)
Conductivity = (g + hf² + if³ + jf⁴)/[10(1 + δt + εp)]
(siemens/meter)
t = temperature (°C); p = pressure (decibars); δ = Ctcor; ε = CPcor
```

Calculating Fluorometry Voltage

```
f = decimal equivalent of bytes 15-17
Fluorometry Voltage = f/819
```

Calculating Transmittance

```
Vdark = 0.058 V
Vref = 4.765 V
t = decimal equivalent of bytes 18 – 20
Transmissometer Voltage (Vsignal) = t/819
% Transmittance = (Vsignal - Vdark) / (Vref - Vdark)
```

PAR

```
raw data = mV  
calibration scale = 6.27 V/(µEinstiens/cm2sec)  
offset (Vdark) = 0.1 mV  
(raw mV - Vdark)/scale x 104 cm2/m2 x 10-3 V/mV = µEinstiens/m2sec  
or  
(data mV - 0.1 mV) x 1.65 (µEinstiens/m2sec)/mV =  
µEinstiens/m2sec
```

PIR

```
raw data = mV  
calibration scale = 4.09 x 10-6 V/(W/m2)  
data mV / (scale x 103 mV/V) = W/m2  
or  
data mV x 242.1(W/m2)/mV = W/m2
```

PSP

```
raw data = mV  
calibration scale = 7.94 x 10-6 V/(W/m2)  
data mV / (scale x 103 mV/V) = W/m2  
or  
data mV x 120.7 (W/m2)/V = W/m2
```

Acquisition Problems and Events

This section lists problems with acquisition noted during this cruise including instrument failures, data acquisition system failures and any other factor affecting this data set. The format is ddd:hh:mm (ddd is year-day, hh is hour, and mm is minute). Times are reported in GMT.

Time	Description
100	Run New_Cruise for NBP0603
	Reboot fram and eltanin
102:12:49	Crossed 68° at: -52 47.321 -67 57.339 Started data collection
102:23:21	Started Knudsen Bathy comparison
102:00:03	Switched to Knudsen
103:01:13	Restart GUV
103:01:28	Switched from Knudsen to Bathy (3.5 only)
103:22:48	Restarted GUV for training
108:23:17	Disabled OS38 cable via sensor.cfg.py for testing. Stopped cruise NBP0603 on ADCP
	Shutdown uhdas
	Started uhdas
	Restarted ADCP as NBP0603A
109:02:06	Re-enabled 0538 after cable test cruise NBP0603B
111:23:56	Bathy 2KW clock error. Set clock back 2 mins to synch with rubidium.
115:04:40	Turned off differential correction to seapath 2
119:	Port wind bird lost propeller. Not repaired due to weather.
120:	The control computer for the Simrad E M120 blew its hard disk. The disk was replaced and the system restored. We were in transit between science areas and no critical data was lost. Total down time was 6 hours.
121:00:30	Ended ADCP cruise NBP0603B Disabled OS38 for trouble shooting. Restarted NBP0603C w/NB150 only
121:01:43	Re-enabled OS38 and started NBP0603D*
121:02:02	Restarted ADCP NBP0603D
126:15:10	Turned off DAS logging and ADCP upon crossing 68°. End of data collection for cruise.
	* OS38 ADCP sonar did not function correctly during NBP0603.

Appendix: Sensors and Calibrations

NBP0603 Sensors:

Shipboard Sensors

Sensor	Description	Serial #	Last Calibration Date	Comments
Meteorology & Radiometers				
Port Anemometer	RM Young 5106	WM46262	12/12/04	
Stbd Anemometer	RM Young 5106	WM51143	10/07/05	
Barometer	RM Young 61201	01706	04/23/05	
Humidity/Wet Temp	RM Young 41372LC	06135	06/24/05	
PIR (Pyrgrometer)	Eppley PIR	32845F3	5/31/05	
PSP (Pyranometer)	Eppley PSP	32850F3	5/31/05	
PAR (Mast)	BSI-QSR-240	6356	05/16/05	
GUV (Mast)	BSI GUV-2511	25110203114	09/07/05	
PUV (Underwater)	BSI PUV-2500	25000203114	09/07/05	
PRR (Mast)	BSI PRR-610	9696	01/09/04	
PRR (Underwater)	BSI PRR-600	9695	01/09/04	
Underway				
TSG	SeaBird SBE21	218091-1390	03/12/05	
TSG Remote Temp	SeaBird 3-01/S	031497	11/10/05	
Fluorometer	Turner 10-AU-005	5333-FRXX	N/A	
Transmissometer	WET Labs C-Star	CST-557DR	04/07/05	
Gravimeter	LaCoste & Romberg Gravity Meter		n/a	Gravity Tie 4/6/06
Bathymetry	Knudsen 320B/R		n/a	
Bathymetry	Bathy 2000		n/a	
Other				
P-Code GPS	Trimble 20636-00 (SM)	0220035116		

NBP0601 CTD Sensors

Sensor	Description	Serial #	Last Calibration Date	Comments
CTD Fish	SeaBird model SBE 9+	09P7536-0328	04/18/05	
CTD Fish Pressure	Paroscientific model 410K-105 pressure sensor	53980	04/18/05	
CTD Deck Unit	SeaBird model SBE 11+	11P19858-0490	n/a	
Primary Temperature Sensor	SeaBird model 3-02/F	032308	11/10/05	
Secondary Temperature Sensor	SeaBird model 3-02/F	032438	11/11/05	
Primary Conductivity Sensor	SeaBird model 4-02/0	041798	04/18/05	
Secondary Conductivity Sensor	SeaBird model 4C	041314	11/11/05	
Dissolved Oxygen Sensor	SeaBird model SBE43	0080	12/3/05	
Transmissometer	WET Labs C-Star	CST-889DR	08/08/05	
CTD Pump (Primary)	SeaBird 5T, PN 90160	050859 3.0K	10/17/04	
CTD Pump (Secondary)	SeaBird 5T, PN 90160	051265 3.0K	12/1/04	
Bottom Contact Switch	SeaBird	#1	n/a	
Altimeter	OIS 6000 (6000m)	497	n/a	
Carousel Water Sampler	SeaBird SBE-32	3214153-0140	n/a	

Calibrations

The following pages are replicas of current calibration sheets for the sensors used during this cruise.

Gravity Tie

Gravity Tie Spreadsheet

The fields outlined in BOLD MUST BE FILLED IN for this spreadsheet to operate properly.
The automatically calculated values show up in the shaded fields.

Date:	4/6/2006	Reference Code Numbers:
Location:	Punta Arenas, Chile	Station no. 9337-50
Station:	Harbour Admin. Bldg.	ISGN no. 51230N
Latitude:	53 09 S	
Longitude:	070 55 W	
Elevation:		
Gravity:	981320.82	

Value	Time (GMT)
Ship's meter before gravity tie (Gravity (cu))	8966.9 12:43
Ship's meter after gravity tie (Gravity (cu))	8967.0 13:39
Average	8967.0
Ship Gravimeter's Calibration Constant	1.0046
Corrected ship's meter (QC Grav (mgal))	9008.2

Value	Time (GMT)
Ship's meter before gravity tie (serial, RVDAS)	8966.9 12:44
Ship's meter after gravity tie (serial, RVDAS)	8966.9 13:40
Average (for comparison check only)	8966.9

Portable Gravimeter Correction Divisor 1.007937

Station	Value	Time (GMT)	Temp	Date
Pier measurement 1	4909.24	12:56	53.5	April 6, 2006
Pier measurement 2	4909.22	12:57	53.5	April 6, 2006
Pier measurement 3	4909.21	13:01	53.5	April 6, 2006
Average	4909.22			

OBS mgal, averaged 4870.57

Station measurement 1	4909.90	13:15	53.5	April 6, 2006
Station measurement 2	4910.00	13:16	53.5	April 6, 2006
Station measurement 3	4909.93	13:21	53.5	April 6, 2006
Average	4909.94			

OBS mgal, averaged 4871.28

Pier measurement 4	4909.31	13:30	53.5	April 6, 2006
Pier measurement 5	4909.30	13:34	53.5	April 6, 2006
Pier measurement 6	4909.34	13:36	53.5	April 6, 2006
Average	4909.32			

OBS mgal, averaged 4870.66

Gravity offset from last tie 972311.96
Drift since last tie 0.29

OBS Differences	Comments
Station to Pier (1, 2, & 3 averaged)	
Station to Pier (4, 5, & 6 averaged)	
Averaged Differences	
Gravity at pier	
Elevation of pier above gravimeter, meters	
Earth differential gravity, mgal/meter	
Gravity at ship's gravimeter	
Gravity Offset (for RVDAS)	

-0.71
-0.62
-0.67
981320.15
1.0
0.3
981320.45
972312.25

Gravity tie completed by Sheldon Blackman and Dan Elsberg at the Punta Arenas, Chile Harbour Administration Bldg. The tie went very smoothly, some oscillations in the needle.

Meteorology System

Anemometer (Port)

RM Young Anemometer Calibration, Model 05106

S/N: 46262

Date: 12-Dec-04

Cal'd By: W. Gallagher

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.0	0.0	0.0
200	0.98	0.9	0.1	1.9
500	2.45	2.3	0.2	4.8
1000	4.90	4.9	0.0	9.5
1500	7.35	7.4	-0.1	14.3
2000	9.80	9.8	0.0	19.0
3000	14.70	14.8	-0.1	28.6
4000	19.60	19.8	-0.2	38.1
5000	24.50	24.8	-0.3	47.6
6000	29.40	29.8	-0.4	57.1
7000	34.30	34.7	-0.4	66.6
8000	39.20	39.8	-0.6	76.2
9000	44.10	44.7	-0.6	85.7
10000	49.00	49.7	-0.7	95.2
12000	58.80	59.5	-0.7	114.2

Direction	Measured Direction	Delta Direction
0	1	0
30	30	0
60	60	0
90	89	1
120	119	1
150	149	1
180	179	1
210	210	0
240	241	-1
270	272	-2
300	302	-2
330	332	-2
0	1	-1

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.0	0.0
200	0.98	0.9	0.1
500	2.45	2.3	0.2
1000	4.90	4.9	0.0
1500	7.35	7.3	0.0
2000	9.80	9.8	0.0
3000	14.70	14.8	-0.1
4000	19.60	19.8	-0.2
5000	24.50	24.8	-0.3
6000	29.40	29.8	-0.4
7000	34.30	34.8	-0.5
8000	39.20	39.8	-0.6
9000	44.10	44.7	-0.6
10000	49.00	49.8	-0.8
12000	58.80	59.7	-0.9

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm? yes
 Wind Direction Threshold < 30 gm? yes

Additional Comments
INSTALLED NEW BEARINGS AND PROPELLER SHAFT. TESTED OKAY

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

Anemometer (Starboard)**RM Young Anemometer Calibration, Model 05106**

S/N: 51143

Date: 07-Oct-05

Cal'd By: J. Lenorovitz

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.00	0.00	0.0
200	0.98	0.90	0.08	1.9
500	2.45	2.35	0.10	4.8
1000	4.90	4.85	0.05	9.5
1500	7.35	7.35	0.00	14.3
2000	9.80	9.80	0.00	19.0
3000	14.70	14.75	-0.05	28.6
4000	19.60	19.75	-0.15	38.1
5000	24.50	24.70	-0.20	47.6
6000	29.40	29.65	-0.25	57.1
7000	34.30	34.65	-0.35	66.6
8000	39.20	39.60	-0.40	76.2
9000	44.10	44.55	-0.45	85.7
10000	49.00	49.50	-0.50	95.2
12000	58.80	59.35	-0.55	114.2

Direction	Measured Direction	Delta Direction
0	0	0
30	30	0
60	60	0
90	90	0
120	120	0
150	150	0
180	180	0
210	208	2
240	239	1
270	269	1
300	300	0
330	330	0
0	0	0

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.00	0.00
200	0.98	0.85	0.13
500	2.45	2.35	0.10
1000	4.90	4.85	0.05
1500	7.35	7.35	0.00
2000	9.80	9.75	0.05
3000	14.70	14.75	-0.05
4000	19.60	19.75	-0.15
5000	24.50	24.70	-0.20
6000	29.40	29.65	-0.25
7000	34.30	34.65	-0.35
8000	39.20	39.55	-0.35
9000	44.10	44.55	-0.45
10000	49.00	49.50	-0.50
12000	58.80	59.35	-0.55

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm? yes
Wind Direction Threshold < 30 gm? yes

Additional Comments

No repairs or adjustments needed. Unit was spot on from the drawer.

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

PIR**THE EPPELEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA
 Telephone: 401-847-1020
 Email: info@eppleylab.com
 Fax: 401-847-1031
 Internet: www.eppleylab.com



Scientific Instruments
for Precision Measurements
Since 1917

**STANDARDIZATION OF
EPPELEY PRECISION INFRARED RADIOMETER
Model PIR**

Serial Number: 32845F3

Resistance: 739 Ω at 23 °C
 Temperature Compensation Range: -20 to 40 °C

This pyrgeometer has been compared against Eppley's Blackbody Calibration System under radiation intensities of approximately 200 watts meter⁻² and an average ambient temperature of 25 °C as measured by Standard Omega Temperature Probe, RTD#1.

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$4.09 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 700 watts meter⁻². This radiometer is linear to within ±1.0% up to this intensity.

The calibration of this instrument is traceable to the International Practical Temperature Scale (IPTS) through a precision low-temperature blackbody.

Shipped to:

National Science Foundation
Port Hueneme, CA

Date of Test: May 31, 2005

In Charge of Test: *R.T. Eppley*

S.O. Number: 60312

Reviewed by: *Thomas D. Kuhn*

Date: June 13, 2005

Remarks:

PSP**THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA

Telephone: 401-847-1020

Fax: 401-847-1031

Email: info@eppleylab.com

Internet: www.eppleylab.com



Scientific Instruments
for Precision Measurements
Since 1917

**STANDARDIZATION
OF
EPPLEY PRECISION SPECTRAL PYRANOMETER
Model PSP**

Serial Number: 32850F3

Resistance: 706 Ω at 23 °C

Temperature Compensation Range: -20 to 40 °C

This radiometer has been compared with Standard Precision Spectral Pyranometer, Serial Number 21231F3 in Eppley's Integrating Hemisphere under radiation intensities of approximately 700 watts meter⁻² (roughly one-half a solar constant). The adopted calibration temperature is 25 °C.

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$7.94 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 1400 watts meter⁻². This radiometer is linear to within ± 0.5% up to this intensity.

The calibration of this instrument is traceable to standard self-calibrating cavity pyrheliometers in terms of the Systems Internationale des Unites (SI units), which participated in the Ninth International Pyrheliometric Comparisons (IPC IX) at Davos, Switzerland in September-October 2000.

Useful conversion facts: 1 cal cm⁻² min⁻¹ = 697.3 watts meter⁻²
1 BTU/ft²-hr⁻¹ = 3.153 watts meter⁻².

Shipped to:
National Science Foundation
Port Hueneme, CA

Date of Test: June 1, 2005

In Charge of Test: *T.G. Gossman*

S.O. Number: 60311
Date: June 13, 2005

Reviewed by: *Thomas J. Kuh*

Remarks:

GUV

GUV-2511 Calibration Certificate																																																																																								
System Serial Number				Date of Calibration				9-07-05																																																																																
Calibration database				Date of Certificate				9/8/2005																																																																																
DASSN				Standard of Spectral Irradiance				99188																																																																																
Microprocessor Tag Number				Operator				TC																																																																																
<table border="1"> <thead> <tr> <th>Monochromatic Channels</th> <th>Address</th> <th>Wavelength [nm]</th> <th>Responsivity [Amps per $\mu\text{W}/(\text{cm}^2\text{nm})$]</th> <th>ScaleSmall [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]</th> <th>ScaleMedium [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]</th> <th>ScaleLarge [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]</th> <th>OffsetSmall [volts]</th> <th>OffsetMedium [volts]</th> <th>OffsetLarge [volts]</th> <th>Measurement Units</th> </tr> </thead> <tbody> <tr> <td>Ed0320</td> <td>2</td> <td>320</td> <td>2.4952E-10</td> <td>2.5451E-05</td> <td>7.4358E-03</td> <td>2.3469E+00</td> <td>-1.5175E-04</td> <td>-1.5535E-04</td> <td>6.9831E-05</td> <td>$\mu\text{W}/(\text{cm}^2\text{nm})$</td> </tr> <tr> <td>Ed0340</td> <td>6</td> <td>340</td> <td>1.9286E-10</td> <td>1.9671E-05</td> <td>5.7471E-03</td> <td>1.9715E+00</td> <td>1.1280E-04</td> <td>1.1544E-04</td> <td>9.0091E-04</td> <td>$\mu\text{W}/(\text{cm}^2\text{nm})$</td> </tr> <tr> <td>Ed0313</td> <td>8</td> <td>313</td> <td>2.3928E-10</td> <td>2.4405E-05</td> <td>7.1299E-03</td> <td>2.5028E+00</td> <td>8.0291E-04</td> <td>7.8935E-03</td> <td>-1.4998E-03</td> <td>$\mu\text{W}/(\text{cm}^2\text{nm})$</td> </tr> <tr> <td>Ed0305</td> <td>10</td> <td>305</td> <td>1.2875E-11</td> <td>1.3133E-06</td> <td>3.8366E-04</td> <td>1.3188E-01</td> <td>2.2863E-04</td> <td>2.3016E-04</td> <td>8.0871E-04</td> <td>$\mu\text{W}/(\text{cm}^2\text{nm})$</td> </tr> <tr> <td>Ed0380</td> <td>12</td> <td>380</td> <td>8.2108E-11</td> <td>8.3750E-06</td> <td>2.4468E-03</td> <td>7.8480E-01</td> <td>2.1481E-04</td> <td>2.0369E-04</td> <td>-2.9957E-04</td> <td>$\mu\text{W}/(\text{cm}^2\text{nm})$</td> </tr> <tr> <td>Ed0395</td> <td>18</td> <td>400-700</td> <td>2.9626E-10</td> <td>3.0218E-05</td> <td>8.8284E-03</td> <td>2.7907E+00</td> <td>2.6231E-04</td> <td>2.6299E-04</td> <td>1.1498E-03</td> <td>$\mu\text{W}/(\text{cm}^2\text{nm})$</td> </tr> </tbody> </table>	Monochromatic Channels	Address	Wavelength [nm]									Responsivity [Amps per $\mu\text{W}/(\text{cm}^2\text{nm})$]	ScaleSmall [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]	ScaleMedium [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]	ScaleLarge [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units	Ed0320	2	320	2.4952E-10	2.5451E-05	7.4358E-03	2.3469E+00	-1.5175E-04	-1.5535E-04	6.9831E-05	$\mu\text{W}/(\text{cm}^2\text{nm})$	Ed0340	6	340	1.9286E-10	1.9671E-05	5.7471E-03	1.9715E+00	1.1280E-04	1.1544E-04	9.0091E-04	$\mu\text{W}/(\text{cm}^2\text{nm})$	Ed0313	8	313	2.3928E-10	2.4405E-05	7.1299E-03	2.5028E+00	8.0291E-04	7.8935E-03	-1.4998E-03	$\mu\text{W}/(\text{cm}^2\text{nm})$	Ed0305	10	305	1.2875E-11	1.3133E-06	3.8366E-04	1.3188E-01	2.2863E-04	2.3016E-04	8.0871E-04	$\mu\text{W}/(\text{cm}^2\text{nm})$	Ed0380	12	380	8.2108E-11	8.3750E-06	2.4468E-03	7.8480E-01	2.1481E-04	2.0369E-04	-2.9957E-04	$\mu\text{W}/(\text{cm}^2\text{nm})$	Ed0395	18	400-700	2.9626E-10	3.0218E-05	8.8284E-03	2.7907E+00	2.6231E-04	2.6299E-04	1.1498E-03	$\mu\text{W}/(\text{cm}^2\text{nm})$			
Monochromatic Channels	Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{W}/(\text{cm}^2\text{nm})$]	ScaleSmall [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]	ScaleMedium [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]	ScaleLarge [Volts per $\mu\text{W}/(\text{cm}^2\text{nm})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units																																																																														
Ed0320	2	320	2.4952E-10	2.5451E-05	7.4358E-03	2.3469E+00	-1.5175E-04	-1.5535E-04	6.9831E-05	$\mu\text{W}/(\text{cm}^2\text{nm})$																																																																														
Ed0340	6	340	1.9286E-10	1.9671E-05	5.7471E-03	1.9715E+00	1.1280E-04	1.1544E-04	9.0091E-04	$\mu\text{W}/(\text{cm}^2\text{nm})$																																																																														
Ed0313	8	313	2.3928E-10	2.4405E-05	7.1299E-03	2.5028E+00	8.0291E-04	7.8935E-03	-1.4998E-03	$\mu\text{W}/(\text{cm}^2\text{nm})$																																																																														
Ed0305	10	305	1.2875E-11	1.3133E-06	3.8366E-04	1.3188E-01	2.2863E-04	2.3016E-04	8.0871E-04	$\mu\text{W}/(\text{cm}^2\text{nm})$																																																																														
Ed0380	12	380	8.2108E-11	8.3750E-06	2.4468E-03	7.8480E-01	2.1481E-04	2.0369E-04	-2.9957E-04	$\mu\text{W}/(\text{cm}^2\text{nm})$																																																																														
Ed0395	18	400-700	2.9626E-10	3.0218E-05	8.8284E-03	2.7907E+00	2.6231E-04	2.6299E-04	1.1498E-03	$\mu\text{W}/(\text{cm}^2\text{nm})$																																																																														
<table border="1"> <thead> <tr> <th>Broadband Channels</th> <th>Address</th> <th>Wavelength [nm]</th> <th>Responsivity [Amps per $\mu\text{E}/(\text{cm}^2\text{s})$]</th> <th>ScaleSmall [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]</th> <th>ScaleMedium [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]</th> <th>ScaleLarge [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]</th> <th>OffsetSmall [volts]</th> <th>OffsetMedium [volts]</th> <th>OffsetLarge [volts]</th> <th>Measurement Units</th> </tr> </thead> <tbody> <tr> <td>Ed0PAR</td> <td>13</td> <td>0</td> <td>1.7094E-05</td> <td>1.7436E+00</td> <td>5.0941E+02</td> <td>1.8003E+05</td> <td>4.1797E-04</td> <td>4.1364E-04</td> <td>-6.9777E-04</td> <td>$\mu\text{E}/(\text{cm}^2\text{sec})$</td> </tr> </tbody> </table>	Broadband Channels	Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{E}/(\text{cm}^2\text{s})$]	ScaleSmall [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]	ScaleMedium [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]	ScaleLarge [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units	Ed0PAR	13	0	1.7094E-05	1.7436E+00	5.0941E+02	1.8003E+05	4.1797E-04	4.1364E-04	-6.9777E-04	$\mu\text{E}/(\text{cm}^2\text{sec})$																																																																		
Broadband Channels	Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{E}/(\text{cm}^2\text{s})$]	ScaleSmall [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]	ScaleMedium [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]	ScaleLarge [Volts per $\mu\text{E}/(\text{cm}^2\text{s})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units																																																																														
Ed0PAR	13	0	1.7094E-05	1.7436E+00	5.0941E+02	1.8003E+05	4.1797E-04	4.1364E-04	-6.9777E-04	$\mu\text{E}/(\text{cm}^2\text{sec})$																																																																														
<table border="1"> <thead> <tr> <th>Auxiliary Channels</th> <th>Address</th> <th>Wavelength</th> <th>Responsivity</th> <th>ScaleS</th> <th>ScaleM</th> <th>ScaleL</th> <th>OffsetS</th> <th>OffsetM</th> <th>OffsetL</th> <th>Measurement Units</th> </tr> </thead> <tbody> <tr> <td>Ed0Temp</td> <td>22</td> <td>0</td> <td>1.0000E+00</td> <td>1.0000E-02</td> <td>1.0000E-02</td> <td>1.0000E-02</td> <td>0.0000E+00</td> <td>0.0000E+00</td> <td>0.0000E+00</td> <td>C</td> </tr> <tr> <td>Ed0Vin</td> <td>27</td> <td>0</td> <td>1.0000E+00</td> <td>-2.5000E-01</td> <td>-2.5000E-01</td> <td>-2.5000E-01</td> <td>0.0000E+00</td> <td>0.0000E+00</td> <td>0.0000E+00</td> <td>V</td> </tr> </tbody> </table>	Auxiliary Channels	Address	Wavelength	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement Units	Ed0Temp	22	0	1.0000E+00	1.0000E-02	1.0000E-02	1.0000E-02	0.0000E+00	0.0000E+00	0.0000E+00	C	Ed0Vin	27	0	1.0000E+00	-2.5000E-01	-2.5000E-01	-2.5000E-01	0.0000E+00	0.0000E+00	0.0000E+00	V																																																							
Auxiliary Channels	Address	Wavelength	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement Units																																																																														
Ed0Temp	22	0	1.0000E+00	1.0000E-02	1.0000E-02	1.0000E-02	0.0000E+00	0.0000E+00	0.0000E+00	C																																																																														
Ed0Vin	27	0	1.0000E+00	-2.5000E-01	-2.5000E-01	-2.5000E-01	0.0000E+00	0.0000E+00	0.0000E+00	V																																																																														

[©] Biospherical Instruments Inc., 5340 Riley Street, San Diego, California 92037 USA. Contact support@biospherical.com for more information.

Calibration Data – Do Not Destroy

page 2 of 2

PUV

PUV-2500 Calibration Certificate										
Calibration factors are immersion corrected for use under water										
System Serial Number			25000203114			Date of Calibration			9-07-05	
Calibration database			25000203114v3.mdb			Date of Certificate			9/6/2005	
DASN			0065			Standard of Spectral Irradiance			99188	
Microprocessor Tag Number			1			Operator			TC	
Monochromatic Channels	Address	Wavelength [nm]	Responsivity [Amps per μW/(cm²·nm)]	ScaleSmall [Volts per μW/(cm²·nm)]	ScaleMedium [Volts per μW/(cm²·nm)]	ScaleLarge [Volts per μW/(cm²·nm)]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
EdZ305	2	305	1.8852E-11	1.9025E-08	5.5583E-04	1.9824E-01	-4.2289E-05	-8.1711E-05	7.8794E-05	μW/(cm²·nm)
EdZ313	5	313	1.4411E-10	1.4700E-05	4.2946E-03	1.5116E+00	1.9947E-04	1.8164E-04	1.7406E-04	μW/(cm²·nm)
EdZ320	6	320	1.3495E-10	1.3765E-05	4.0216E-03	1.2480E+00	3.2945E-04	3.1244E-04	4.1357E-04	μW/(cm²·nm)
EdZ395	10	395	2.3525E-10	2.3995E-05	7.0104E-03	2.1867E+00	1.3688E-04	1.1986E-04	1.6849E-04	μW/(cm²·nm)
EdZ340	11	340	1.0900E-10	1.1118E-05	3.2481E-03	1.0931E+00	1.9811E-04	1.8545E-04	5.1597E-04	μW/(cm²·nm)
EdZ380	18	400-700	6.1932E-11	6.3171E-06	1.8456E-03	8.6997E-01	-1.7272E-04	-1.9269E-04	-1.8676E-03	μW/(cm²·nm)
Broadband Channels	Address	Wavelength [nm]	Responsivity [Amps per μE/(cm²·s)]	ScaleSmall [Volts per μE/(cm²·s)]	ScaleMedium [Volts per μE/(cm²·s)]	ScaleLarge [Volts per μE/(cm²·s)]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
EdZPAR	14	0	1.7708E-05	1.8062E+00	5.2770E+02	1.6687E+05	-2.5409E-04	-2.7288E-04	-2.3886E-03	μE/(cm²·sec)
LuZChl	15	0	5.4318E-11	5.5405E-06	1.6187E-03	5.7788E-01	7.8880E-05	5.7578E-05	-4.3020E-05	nE/(sr·m²·sec)
Auxiliary Channels	Address	Wavelength	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement
EdZGnd	0	0	1	1.0000	1.0000	1.0000	0.0000	0.0000	0.0000	amps
WTemp	20	0	1.0000E+00	1.8982E-01	1.8982E-01	1.8982E-01	4.3925E-02	4.3925E-02	4.3925E-02	C
Depth	21	0	1.0000E+00	2.5533E-02	2.5533E-02	2.5533E-02	2.8643E-01	2.8643E-01	2.8643E-01	m
EdZTemp	22	0	1.0000E+00	1.0000E-02	1.0000E-02	1.0000E-02	0.0000E+00	0.0000E+00	0.0000E+00	C
LuZTemp	23	0	1.0000E+00	1.0000E-02	1.0000E-02	1.0000E-02	0.0000E+00	0.0000E+00	0.0000E+00	C
Tilt	24	0	1.0000E+00	3.7504E-02	3.7504E-02	3.7504E-02	3.4409E+00	3.4409E+00	3.4409E+00	"
Roll	25	0	1.0000E+00	3.4985E-02	3.4985E-02	3.4985E-02	3.5475E+00	3.5475E+00	3.5475E+00	"
EdZVin	27	0	1.0000E+00	-2.5000E-01	-2.5000E-01	-2.5000E-01	0.0000E+00	0.0000E+00	0.0000E+00	V

Calibration Data - Do Not Destroy

page 2 of 3

PAR**Biospherical Instruments Inc.**

CALIBRATION CERTIFICATE

Calibration Date 5/16/2005
 Model Number QSR-240
 Serial Number 6356
 Operator TPC
 Standard Lamp 99189(4/12/05)
 Probe Excitation Voltage Range: 6 to 18 VDC(+)
 Output Polarity: POSITIVE

Probe Conditions at Calibration(in air):

Calibration Voltage: 6 VDC(+)
 Probe Current: 1.2 mA

Probe Output Voltage:

Probe Illuminated 86.9 mV
 Probe Dark 0.1 mV
 Probe Net Response 86.8 mV

Corrected Lamp Output:

Output In Air (same condition as calibration):

8.34E+15 quanta/cm²sec
0.01384 uE/cm²sec

Calibration Factor:

(To calculate irradiance, divide the net voltage reading in Volts by this value.)

Dry: 1.04E-17 V/(quanta/cm²sec)
6.27E+00 V/(uE/cm²sec)

Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with alcohol.
4. Calibration was performed with customer cable, when available.

TSG Calibration Files

Underway Conductivity

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1390
 CALIBRATION DATE: 12-Mar-05

SBE21 CONDUCTIVITY CALIBRATION DATA
 PSS 1978: C(35,15,0) = 4.2914 Seimens/meter

GHIJ COEFFICIENTS

g = -3.93226726e+000
 h = 4.70569719e-001
 i = 6.34631789e-004
 j = -9.87772523e-006
 CPcor = -9.5700e-008 (nominal)
 CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 4.43616567e-003
 b = 4.64684698e-001
 c = -3.92316496e+000
 d = -8.75063759e-005
 m = 2.4
 CPcor = -9.5700e-008 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2.88539	0.00000	0.00000
0.9999	34.7900	2.97392	8.41759	2.97392	-0.00000
4.5000	34.7690	3.28070	8.79114	3.28070	-0.00000
14.9999	34.7244	4.26152	9.89031	4.26154	0.00002
18.5000	34.7146	4.60633	10.24842	4.60632	-0.00002
24.0000	34.7039	5.16375	10.80209	5.16377	0.00001
29.0000	34.6989	5.68525	11.29521	5.68522	-0.00003
32.5000	34.6969	6.05752	11.63436	6.05754	0.00002

$$\text{Conductivity} = (g + hf^2 + ir^3 + jt^4) / 10(1 + \delta t + \epsilon p) \text{ Siemens/meter}$$

$$\text{Conductivity} = (af^{10} + bf^2 + c + dt) / [10 (1 + \epsilon p)] \text{ Siemens/meter}$$

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

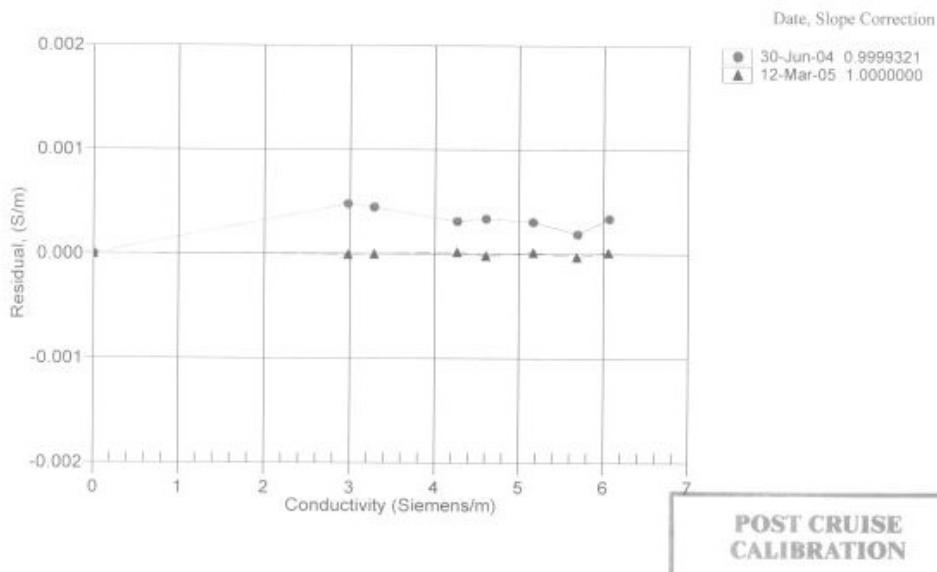

Underway Temperature Sensor

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1390
CALIBRATION DATE: 12-Mar-05

SBE21 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPRATURE SCALE

ITS-90 COEFFICIENTS

g = 4.21050756e-003
b = 5.95355230e-004
i = 4.97876949e-006
j = -1.73798388e-006
f0 = 1000.0

ITS-68 COEFFICIENTS

a = 3.64763867e-003
b = 5.81216773e-004
c = 9.98586302e-006
d = -1.73747972e-006
f0 = 2600.263

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
0.9999	2600.263	0.9997	-0.00018
4.5000	2814.731	4.5003	0.00033
14.9999	3533.537	14.9996	-0.00033
18.5000	3799.663	18.5000	0.00004
24.0000	4245.995	24.0001	0.00012
29.0000	4682.732	29.0002	0.00018
32.5000	5006.584	32.4998	-0.00016

$$\text{Temperature ITS-90} = 1/(g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]) - 273.15 \text{ (}^\circ\text{C)}$$


$$\text{Temperature ITS-68} = 1/(a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]) - 273.15 \text{ (}^\circ\text{C)}$$

Following the recommendation of JPOTS: T_{68} is assumed to be $1.00024 * T_{90}$ (-2 to 35 $^\circ\text{C}$)

Residual = instrument temperature - bath temperature

Date, Offset(mdeg C)

● 30-Jun-04 1.17
▲ 12-Mar-05 -0.00

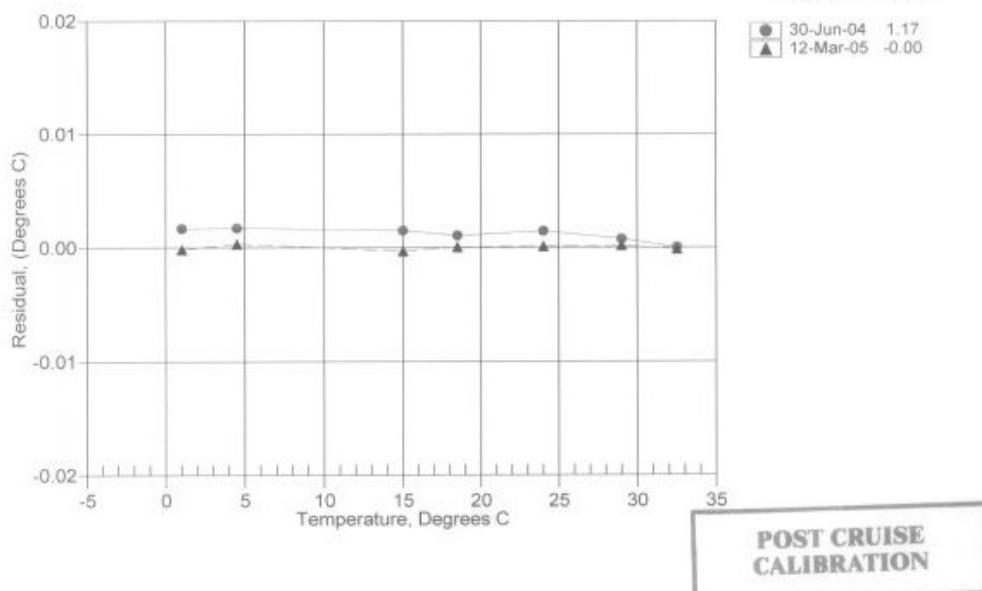

Underway Remote Temperature Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1497
CALIBRATION DATE: 10-Nov-05SBE3 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPRATURE SCALE

ITS-90 COEFFICIENTS

 $a = 4.73766449e-003$
 $b = 6.68793556e-004$
 $c = 2.84645709e+005$
 $d = 2.61326034e-006$
 $e_0 = 1000.0$

ITS-68 COEFFICIENTS

 $a = 3.69121909e-003$
 $b = 5.95381666e-004$
 $c = 1.53096888e-005$
 $d = 2.61478510e-006$
 $e_0 = 3372.992$

BATH TEMP (ITS-90)	INSTRUMENT FREO (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5004	5372.992	-1.5005	-0.00010
0.9996	5685.203	0.9997	0.00005
4.4996	6144.063	4.4997	0.00010
7.9996	6628.986	7.9996	0.00004
11.4996	7140.871	11.4995	-0.00006
14.9996	7679.800	14.9995	-0.00015
18.4996	8247.050	18.4995	-0.00005
21.9996	8843.015	21.9996	0.00002
25.4996	9468.305	25.4997	0.00013
28.9996	10123.458	28.9997	0.00012
32.4996	10808.995	32.4995	-0.00013


$$\text{Temperature ITS-90} = 1/[g + h(\ln(f_0/f))] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)] - 273.15 \text{ (°C)}$$

$$\text{Temperature ITS-68} = 1/[a + b(\ln(f_0/f))] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)] - 273.15 \text{ (°C)}$$

Following the recommendation of JPOTS: T_{hk} is assumed to be $1.00024 * T_{90}$ (-2 to 35 °C)

Residual = instrument temperature - bath temperature

Date, Offset(mdeg C)

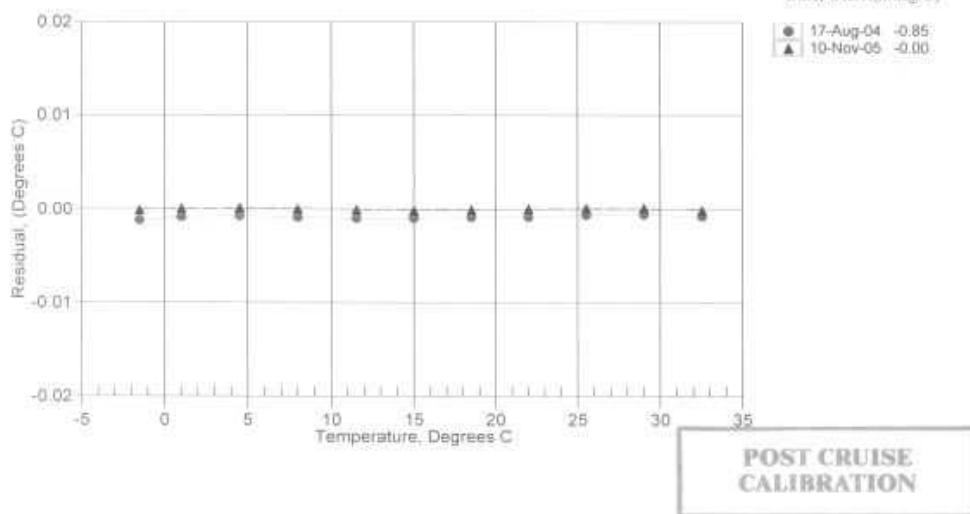

Underway Transmissometer

PO Box 518
620 Applegate St.
Philomath, OR 97370



(541) 929-5650
Fax (541) 929-5277
www.wetlabs.com

C-Star Calibration

Date April 7, 2005	Customer Raytheon Polar Service Co.	Work order 005
Job # 0201020	S/N# CST-557DR	Pathlength 25 cm

Analog meter	
V_d	0.060 V
V_{air}	4.851 V
V_{ref}	4.732 V

Temperature of calibration water	20.0 °C
Ambient temperature during calibration	23.4 °C

Relationship of transmittance (Tr) to beam attenuation coefficient (c), and pathlength (x): $Tr = e^{-cx}$

To determine beam transmittance: $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient: $c = -1/x * \ln(Tr)$

V_d Meter output with the beam blocked. This is the offset.

V_{air} Meter output in air with a clear beam path.

V_{ref} Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain V_{ref}

Ambient temperature: meter temperature in air during the calibration.

V_{sig} Measured signal output of meter.

CTD SENSORS

CTD Fish Pressure Sensor

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0328
CALIBRATION DATE: 18-Apr-05

SBE9plus PRESSURE CALIBRATION DATA
10000 psia S/N 53980


DIGIQUARTZ COEFFICIENTS:
C1 = -5.847002e+004
C2 = 6.910390e-001
C3 = 1.7533360e-002
D1 = 4.241600e-002
D2 = 0.000000e+000
T1 = 3.026040e-001
T2 = -1.938830e-004
T3 = 4.330190e-006
T4 = 2.020250e-009
T5 = 0.000000e+000

AD590M, AD590B, SLOPE AND OFFSET:
AD590M = 1.13300e-002
AD590B = -8.47592e+000
Slope = 1.00004
Offset = -0.7426 (dbars)

PRESSURE (PSIA)	INST OUTPUT(Hz)	INST TEMP(C)	INST OUTPUT(PSIA)	CORRECTED INST OUTPUT(PSIA)	RESIDUAL (PSIA)
14.762	33053.29	22.0	15.752	14.675	-0.087
2014.939	33613.14	23.1	2015.888	2014.886	-0.053
4014.919	34162.20	23.1	4015.804	4014.878	-0.041
6014.986	34701.06	23.2	6015.837	6014.986	-0.000
8014.992	35230.18	23.2	8015.861	8015.085	0.093
10015.554	35749.99	23.2	10015.800	10015.099	-0.455
8014.880	35230.20	23.3	8015.894	8015.117	0.237
6014.818	34701.08	23.3	6015.881	6015.030	0.212
4014.816	34162.23	23.3	4015.923	4014.996	0.180
2014.828	33613.16	23.3	2015.925	2014.923	0.095
14.761	33053.25	23.4	15.657	14.580	-0.181

Residual = corrected instrument pressure - reference pressure

Date, Avg Offset (psia)

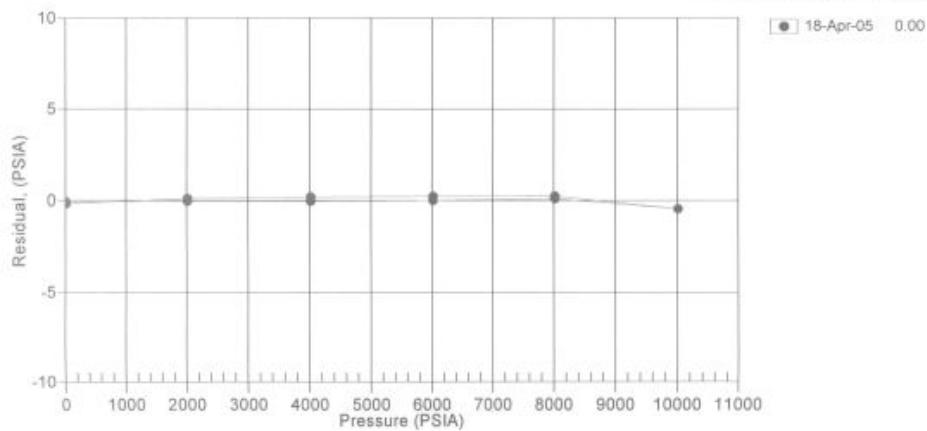

CTD Temperature (Primary)

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA
 Phone: (425) 643 - 9886 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2308
 CALIBRATION DATE: 10-Nov-05

SBE3 TEMPERATURE CALIBRATION DATA
 ITS-90 TEMPRATURE SCALE

ITS-90 COEFFICIENTS

$g = 4.34522472e-003$
 $h = 6.44893405e-004$
 $i = 2.34595443e-005$
 $j = 2.22310880e-006$
 $f_0 = 1000.0$

ITS-68 COEFFICIENTS

$a = 3.68121777e-003$
 $b = 6.02574282e-004$
 $c = 1.63719266e-005$
 $d = 2.22467863e-006$
 $f_0 = 2906.253$

BATH TEMP (ITS-90)	INSTRUMENT FREO (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5004	2906.253	-1.5004	-0.00000
0.9996	3073.056	0.9996	0.00002
4.4996	3318.066	4.4996	-0.00004
7.9996	3576.835	7.9996	0.00001
11.4996	3849.721	11.4996	0.00001
14.9996	4137.086	14.9996	0.00001
18.4996	4439.279	18.4996	0.00001
21.9996	4756.635	21.9996	-0.00001
25.4996	5089.484	25.4996	0.00001
28.9996	5438.128	28.9996	-0.00003
32.4996	5802.880	32.4996	0.00002


$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 (\text{°C})$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 (\text{°C})$$

Following the recommendation of JPOTS: T_{ts} is assumed to be $1.00024 * T_{90}$ (-2 to 35 °C)

Residual = instrument temperature - bath temperature

Date, Offset(mdeg C)

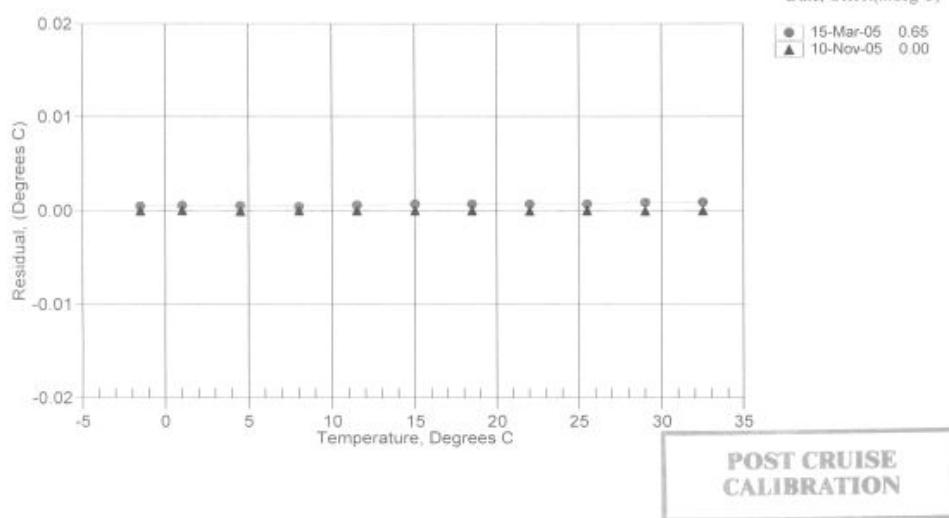

CTD Temperature (Secondary)

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2438
CALIBRATION DATE: 11-Nov-05

SBE3 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPRATURE SCALE

ITS-90 COEFFICIENTS

$g = 4.31128806e-003$
 $h = 6.41856807e-004$
 $i = 2.29752545e-005$
 $j = 2.17699323e-006$
 $f_0 = 1000.0$

ITS-68 COEFFICIENTS

$a = 3.68121754e-003$
 $b = 6.02092337e-004$
 $c = 1.63740991e-005$
 $d = 2.17855606e-006$
 $f_0 = 2759.290$

BATH TEMP (ITS-90)	INSTRUMENT FREO (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5004	2759.290	-1.5004	0.00001
0.9996	2917.786	0.9996	-0.00001
4.4996	3150.616	4.4996	-0.00002
7.9996	3396.532	7.9996	-0.00002
11.4996	3655.890	11.4996	0.00002
14.9996	3929.030	14.9996	0.00005
18.4996	4216.280	18.4996	-0.00000
21.9996	4517.972	21.9996	-0.00002
25.4996	4834.416	25.4996	-0.00002
28.9996	5165.910	28.9996	-0.00002
32.4996	5512.746	32.4996	0.00002


$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ } ^\circ\text{C}$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ } ^\circ\text{C}$$

Following the recommendation of JPOTS: T_{68} is assumed to be $1.00024 * T_{90}$ (-2 to 35 $^\circ\text{C}$)

Residual = instrument temperature - bath temperature

Date, Offset(mdeg C)

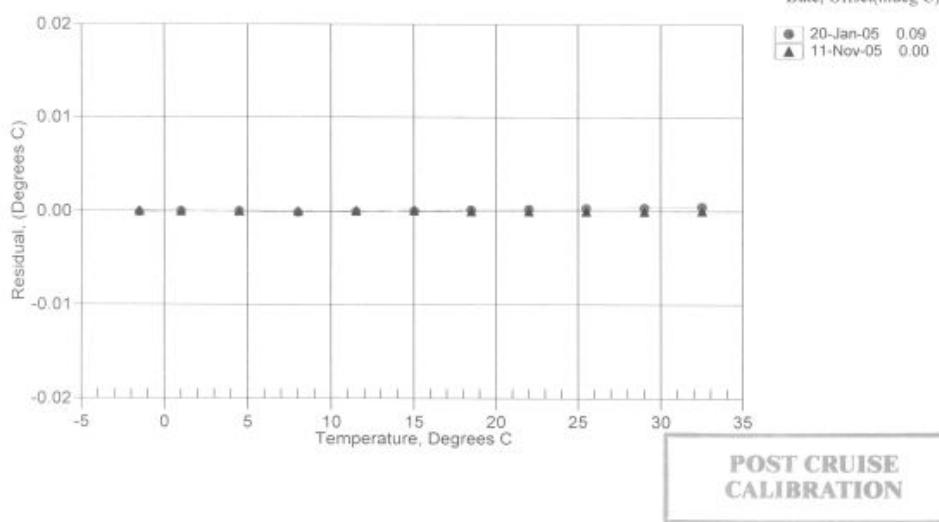

CTD Conductivity (Primary)

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1798
CALIBRATION DATE: 10-Nov-05

SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHU COEFFICIENTS

$g = -4.12046333e+000$
 $h = 4.81408174e-001$
 $i = -5.15924015e-004$
 $j = 5.14576250e-005$
 $CPcor = -9.5700e-008$ (nominal)
 $CTcor = 3.2500e-006$ (nominal)

ABCDM COEFFICIENTS

$a = 1.70695760e-006$
 $b = 4.79615163e-001$
 $c = -4.11453964e+000$
 $d = -8.59014813e-005$
 $m = 5.0$
 $CPcor = -9.5700e-008$ (nominal)

BATH TEMP (ITS-90)	BATH SAL. (PSU)	BATH COND (Siemens/m)	INST FREO (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.92886	0.00000	0.00000
-0.9771	34.9382	2.81542	8.19458	2.81549	0.00006
1.0793	34.9387	2.99232	8.41542	2.99230	-0.00002
14.9999	34.9394	4.28510	9.87862	4.28494	-0.00016
18.4999	34.9379	4.63274	10.23599	4.63281	0.00007
28.9999	34.9346	5.71950	11.27787	5.71970	0.00020
32.4999	34.9253	6.09283	11.61321	6.09269	-0.00014


$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p) \text{ Siemens/meter}$$

$$\text{Conductivity} = (af^0 + bf^2 + c + dt) / [10(1 + \epsilon p)] \text{ Siemens/meter}$$

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

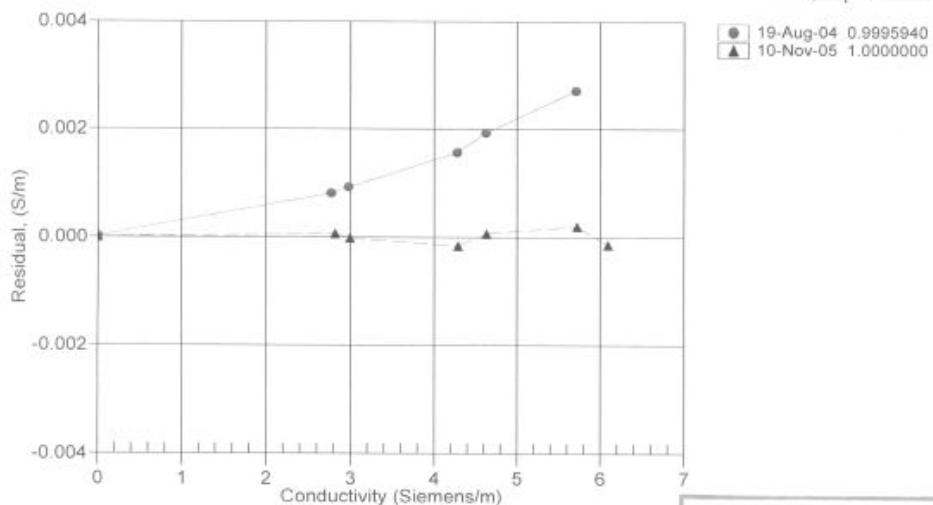

POST CRUISE
CALIBRATION

CTD Conductivity (Secondary)

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA
Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2513
CALIBRATION DATE: 10-Nov-05

SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHIJ COEFFICIENTS

$g = -1.05792413e+001$
 $h = 1.63052186e+000$
 $i = -9.01357414e-004$
 $j = 1.81302971e-004$
 $CPcor = -9.5700e-008$ (nominal)
 $CTcor = 3.2500e-006$ (nominal)

ABCDM COEFFICIENTS

$a = 2.71931735e-005$
 $b = 1.62864947e+000$
 $c = -1.05763881e+001$
 $d = -8.53773538e-005$
 $m = 4.6$
 $CPcor = -9.5700e-008$ (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREO (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.54808	0.00000	0.00000
-0.9771	34.9382	2.81542	4.87406	2.81542	-0.00000
1.0793	34.9387	2.99232	4.98398	2.99233	0.00001
14.9999	34.9394	4.28510	5.72313	4.28506	-0.00004
18.4999	34.9379	4.63274	5.90605	4.63278	0.00004
28.9999	34.9346	5.71950	6.44402	5.71949	-0.00000
32.4999	34.9253	6.09283	6.61865	6.09283	-0.00000

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p) \text{ Siemens/meter}$$

$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10 (1 + \epsilon p)] \text{ Siemens/meter}$$

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

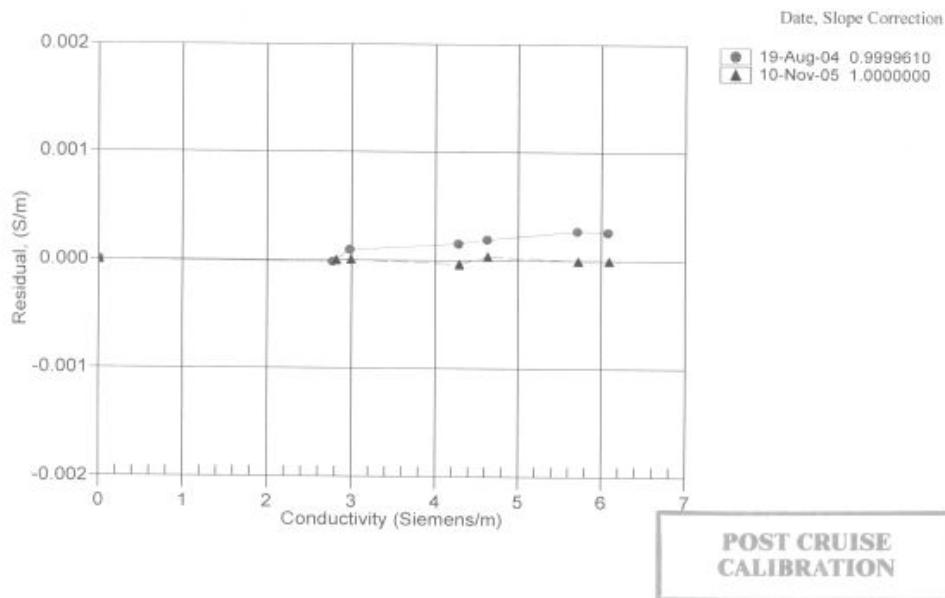

CTD Fluorometer

PO Box 518
820 Applegate St.
Philomath OR 97370



(541) 929-5650
Fax (541) 929-5277
<http://www.wetlabs.com>

Chlorophyll Fluorometer Incoming Characterization

Date: 02/01/06
Serial #: AFLT-009
Job #: 0009099
Tech: K.C.

Dark (Vblank) 0.198 volts
CEV 2.772 volts
SF 9.7125

FSV 5.45 volts

Linearity: 0.999 R² (0–1.5 volts)
0.995 R² (0– 5.45 volts)

Notes:

Dark Counts: Signal output of the meter in clean water with black tape over detector.

CEV is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to 25 µg/l of a *Thalassiosira weissflogii* phytoplankton culture.

SF is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determine by using the following equation:
SF = (25) / (CEV – Dark) e.g.(25 / (2.865 – 0.238) = 9.516)

FSV is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m³) can be derived by using the following equation: (µg/l) = (Vmeasured – CWO) * SF

The relationship between fluorescence and chlorophyll-a concentrations in-situ is high variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by American Public Health Association, American Water Works Association and Water Environment Federation.

CTD Transmissometer

Transmissometer, Chelsea/Seatech/Wetlab	
Serial Number	507014
Calibration Date	8/8/2005
M	21.510
B	-1.194
Path length [m]	0.250
<input type="button" value="OK"/> <input type="button" value="Cancel"/>	

Instructions: Fill out the Blue parts, print it out.
Fill out the SeaSave form so it looks like this.

From Calibration Sheet

Serial Number	507014
Cal Date:	8/8/2005
Vd	0.061
Vair	4.808
Vref	4.687
Pathlength (cm)	25

From On-CTD Pre-Cruise Measurements

Voltage in Air	4.764
Voltage Dark	0.0555

CTD Dissolved Oxygen Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9886 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0080
CALIBRATION DATE: 03-Dec-05p

SBE 43 OXYGEN CALIBRATION DATA

COEFFICIENTS

Soc = 0.3408

TCor = 0.0020

Boc = 0.0000

PCor = 1.350e-04

Voffset = -0.5153

BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.26	2.01	0.00	0.892	1.24	-0.02
1.26	12.00	0.00	1.011	1.31	0.05
1.26	6.00	0.00	0.943	1.28	0.02
1.30	20.00	0.00	1.108	1.34	0.04
1.32	26.00	0.00	1.168	1.33	0.01
1.34	30.00	0.00	1.211	1.33	-0.01
4.17	2.04	0.00	1.742	4.06	-0.11
4.18	6.00	0.00	1.908	4.18	0.00
4.21	12.00	0.00	2.149	4.30	0.09
4.22	20.00	0.00	2.416	4.29	0.07
4.27	26.00	0.00	2.613	4.27	-0.00
4.32	30.00	0.00	2.734	4.24	-0.08
6.90	30.00	0.00	4.052	6.76	-0.14
6.92	2.05	0.00	2.560	6.75	-0.17
6.96	6.00	0.00	2.840	6.98	0.02
6.97	12.01	0.00	3.225	7.13	0.16
6.97	26.00	0.00	3.934	6.96	-0.01
6.99	20.00	0.00	3.668	7.11	0.12

oxygen (ml/l) = (Soc * (V + Voffset)) * exp(Tcor * T) * Oxsat(T,S) * exp(PCor * P)

V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU]

Oxsat(T,S) = oxygen saturation [ml/l], P = pressure [dbar]

Residual = instrument oxygen - bath oxygen

