


# **Data Report NBP0808: FOODBANCS 2**

**Antarctic Peninsula**

**Dr. David DeMaster & Dr. Craig Smith**

**July 10 – August 4, 2008**

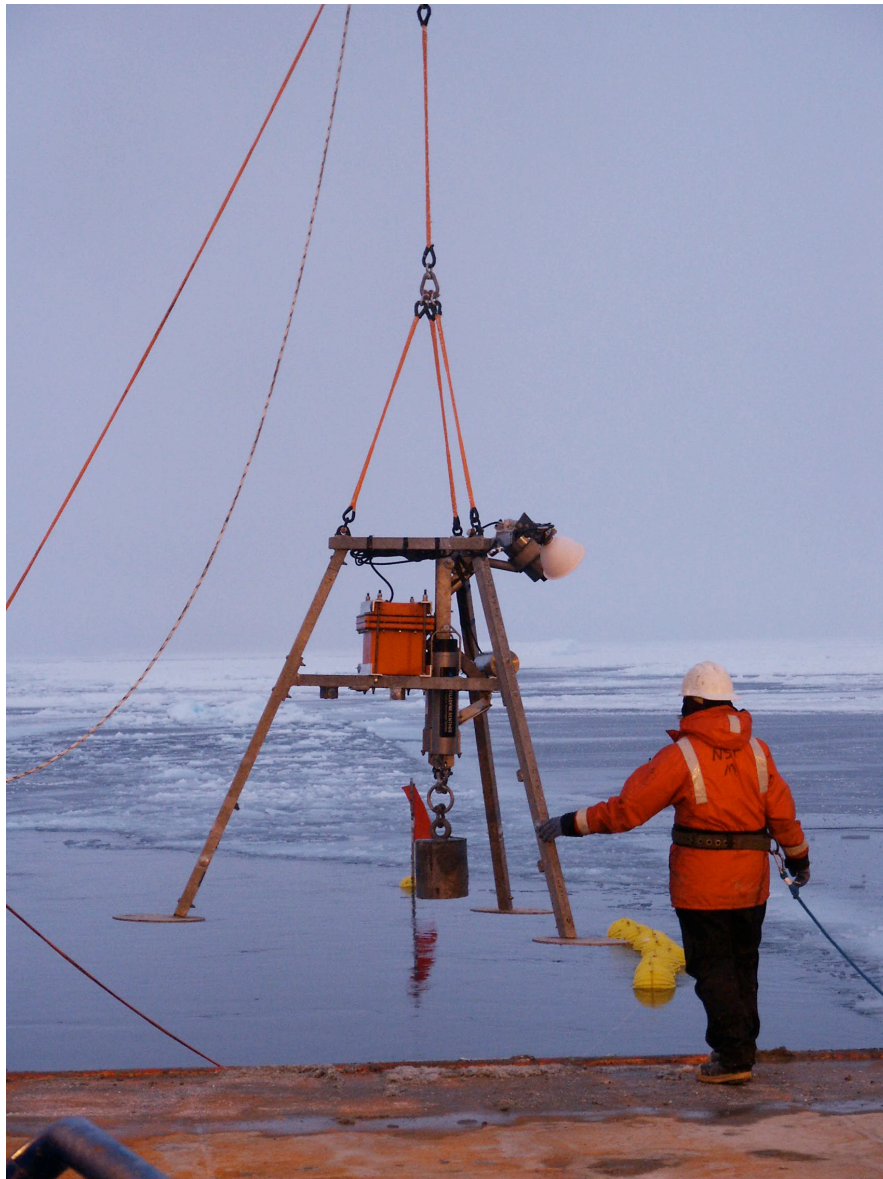

**United States Antarctic Program**

**RVIB Nathaniel B. Palmer**

**Raytheon Polar Services**

**Prepared by Kris Merrill and Jennifer Ayers**

## Table of Contents

<b>INTRODUCTION .....</b>	<b>1</b>
<b>DISTRIBUTION CONTENTS AT A GLANCE .....</b>	<b>2</b>
EXTRACTING DATA .....	3
<b>DISTRIBUTION CONTENTS .....</b>	<b>4</b>
CRUISE INFORMATION .....	4
<i>Cruise Track</i> .....	4
<i>Satellite Images</i> .....	4
NBP DATA PRODUCTS .....	4
<i>JGOFS</i> .....	5
<i>MGD77</i> .....	6
SCIENCE OF OPPORTUNITY .....	7
<i>ADCP</i> .....	7
<i>pCO<sub>2</sub></i> .....	7
CRUISE SCIENCE .....	8
<i>CTD</i> .....	8
RVDAS .....	8
<i>Sensors and Instruments</i> .....	8
Underway Sensors .....	9
Meteorology and Radiometry .....	9
Geophysics .....	9
Oceanography .....	9
Navigational Instruments.....	10
<i>Data</i> .....	10
Underway Data .....	11
Sound Velocity Probe (svp1) .....	11
Meteorology (met1) .....	11
Knudsen (knud).....	11
Thermosalinograph (tsg1) .....	12
Fluorometer (flr1).....	12
pCO <sub>2</sub> (pco2).....	12
Engineering (eng1).....	13
Hydro-DAS (hdas) .....	13
Micro-TSG (mtsg).....	13
GUV Data (pguv).....	14
Remote Temperature (rtmp).....	14
Ultrasonic Anemometer (wind).....	14
Navigational Data .....	15
Seapath GPS (seap).....	15
Trimble (P-Code) GPS (PCOD).....	19
Gyro Compass (gyr1).....	21
Sound Velocity Probe (svp1) .....	21
ADCP Course (adcp).....	22
Processed Data.....	22
pCO <sub>2</sub> -merged .....	22
tsgfl.....	23
<b>CALCULATIONS .....</b>	<b>24</b>
TSG .....	24
PAR .....	24
PSP .....	25
PIR .....	25
<b>ACQUISITION PROBLEMS AND EVENTS .....</b>	<b>26</b>

<b>APPENDIX: SENSORS AND CALIBRATIONS</b>	<b>27</b>
NBP0808 Shipboard Sensors:	27
METEOROLOGY & RADIOMETERS	27
UNDERWAY	27
NBP0808 CTD Sensors:	28
CALIBRATIONS	28
Gravity Tie Start (Punta Arenas)	29
METEOROLOGY SYSTEM	30
Anemometer (Port)	30
Anemometer (Starboard)	31
Anemometer (Bridge)	32
Barometer	33
Humidity Sensor	34
Temperature Sensor	35
PIR	36
PSP	37
PAR	38
GUV	39
TSG CALIBRATION FILES	40
Underway Conductivity	40
Underway Temperature Sensor	41
Underway Temperature Sensor (Primary Remote)	42
Underway Temperature Sensor (Secondary Remote)	43
MICRO-TSG CALIBRATION FILES	44
Temperature Sensor (Micro-TSG)	44
Conductivity Sensor (Micro-TSG)	44
Underway fluorometer (Primary)	45
CTD Pressure Sensor (fish)	47
CTD Primary Temperature Sensor	48
CTD Secondary Temperature Sensor	50
CTD Primary Conductivity Sensor	52
CTD Secondary Conductivity Senesor (cast 007 – on)	55
CTD Primary Dissolved Oxygen Sensor	57
CTD Secondary Dissolved Oxygen Sensor	58
CTD Fluorometer	59
CTD Transmissometer	60

## Introduction

The NBP data acquisition systems continuously log data from the instruments used during the cruise. This document describes:

- The structure and organization of the data on the distribution media
- The format and contents of the data strings
- Formulas for calculating values
- Information about the specific instruments in use during the cruise
- A log of acquisition problems and events during the cruise that may affect the data
- Scanned calibration sheets for the instruments in use during the cruise.

The data is distributed on a DVD-R or CD-ROM written in ISO9660 level-1 format. It is readable by virtually every computing platform.

All the data has been compressed using Unix “gzip,” identified by the “.gz” extension. It has been copied to the distribution media in the Unix tar archive format, “.tar” extension. Tools are available on all platforms for uncompressing and de-archiving these formats: On Macintosh, use Stuffit Expander with DropStuff. On Windows operating systems use WinZip.

MultiBeam and BathyW data, if collected, are distributed separately.

*IMPORTANT: Read the last section, “Acquisition Problems and Events,” for important information that may affect the processing of this data.*



## Distribution Contents at a Glance

Volume 1 of 1: NBP0808		Description
File		
/		Root level directory
	NBP0808.trk	Text file of cruise track (lat,lon)
	NBP0808.mgd	Full Cruise MGD77 data file
	NBP0808.gmt	GMT binary file of MGD77 data
	Instrument_coeff.txt	Instrument Coefficient File
	0808_DataReport.doc	Data Report NBP0808
/plots		Cruise track plots
	0808_Track.ps	Cruise track plot (PostScript format)
	0808_Track.jpg	Cruise track plot (JPEG format)
/process		Geop data
	0808jgof.tar	JGOFS format data files
	0808qc.tar	Daily RVDAS QC postscript plots
	0808pco2.tar	Merged pCO2 data files
	0808mgd.tar	MGD Data
	0808proc.tar	Other processed data
/rvdas/nav		Navigation data
	0808gyr1.tar	Gyro raw data
	0808PCOD.tar	Trimble P-code raw data
	0808seap.tar	Seapath data
	0808adcp.tar	ADCP Data Sets
	0808gp02	Gp02 Data
	0808sp2a.tar	Seapath 2 data
/rvdas/uw		Underway data
	0808bwnc.tar	Baltic Winch raw data
	0808swnc.tar	Starboard Winch raw data
	0808uwnc.tar	Upper Waterfall Winch raw data
	0808flr1.tar	Fluorometer raw data
	0808grv1.tar	Gravimeter raw data
	0808met1.tar	Meteorology raw data
	0808pco2.tar	pCO2 raw data
	0808wind.tar	Ultrasonic anemometer raw data
	0808tsg1.tar	TSG raw data
	0808svp1.tar	Sound velocity probe (in ADCP well)
	0808mtsg.tar	Micro TSG data
	0808eng1.tar	Engineering Data and PIR
	0808hdas.tar	HydroDAS raw data
	0808pguv.tar	GUV raw data
	0808rtmp.tar	Remote temperature data
	0808knud.tar	Knudsen raw data
	0808ctdd.tar	CTD Depth
/Imagery		
	0808Imag.tar	
/ocean		
	0808ctd.tar	

## Extracting Data

The Unix tar command has many options. It is often useful to know exactly how an archive was produced when expanding its contents. All archives were created using the command,

```
tar cvf archive_filename files_to_archive
```

To create a list of the files in the archive, use the Unix command,

```
tar tvf archive_filename > contents.list
```

where `contents.list` is the name of the file to create

To extract the files from the archive:

```
tar xvf archive_filename file(s)_to_extract
```

G-zipped files will have a “.gz” extension on the filename. These files can be decompressed after de-archiving, using the Unix command,

```
gunzip filename.gz
```

## Distribution Contents

### Cruise Information

NBP0808 departed Punta Arenas, Chile on July 10, 2008. There were no major problems during the transit and no instruments changed. The weather and the seas were very cooperative for most of the cruise. We occupied six stations between Elephant Island (61°S) and Marguerite Bay (68°S), conducting over-the side sampling operations using coring techniques (megacorer, box corer, and kasten corer), bottom trawls (Blake Trawls and Otter trawls), CTD profiles, and bottom camera studies (MUD SCUD).

We collected this data to measure benthic faunal feeding strategies and benthic carbon fluxes during winter conditions as part of our 3-cruise field program. The measurements will be used to assess the benthic response to changes in surface carbon production rates as they are affected by global climate change. NBP0808 returned to Punta Areas on August 4.

### Cruise Track

The distribution DVD includes a GMT cruise track file (NBP0808.trk). It contains the longitude and latitude at one-minute intervals extracted from the NBP0808.gmt file.

JPEG and PostScript cruise track files have been produced and placed in the /plots directory.

### Satellite Images

Satellite Images received for this cruise can be found in the file called /Imagery/0808Imag.tar collected and processed on the ship is in two further subdirectories, Ice and WX (weather). Files are named using the convention, ssss\_fff\_mmddyy\_tttt\_ww.gif where:

ssss_fff	= satellite and flight number
mm	= month
dd	= day
yy	= year
tttt	= time in hours and minutes (UTC)
ww	= optional field for identifying wavelength, such as vis (visible) or IR (infrared)

### NBP Data Products

Two datasets are created on each cruise: JGOFS and MGD77.

The data processing scripts used to produce JGOFS and MGD77 data sets create a lot of intermediate files. These files are included on the data distribution media in a file called /process/0808proc.tar. They are included to make re-processing easier in the event of an error, but no extensive detail of the formats is included in this document. If you have any questions, please contact [itvessel@usap.gov](mailto:itvessel@usap.gov).

## JGOFS

The JGOFS data set can be found on the distribution media in the file /process/0808jgof.tar. The archive contains one file produced for each day named jgDDD.dat.gz, where DDD is the year-day the data was acquired. The “.gz” extension indicates that the individual files are compressed before archiving. Each daily file consists of 22 columnar fields in text format as described in the table below. The JGOFS data set is created from calibrated data decimated at one-minute intervals. Several fields are derived measurements from more than a single raw input. For example, Course Made Good (CMG) and Speed Over Ground (SOG) are calculated from gyro and GPS inputs. Daily plots during the cruise are produced from the JGOFS data set. Note: Null, unused, or unknown fields are indicated as “NAN” as 9999 in the JGOFS data.

Field	Data	Units
01	GMT date	dd/mm/yy
02	GMT time	hh:mm:ss
03	NGL latitude (negative is South)	tt.tttt
04	NGL longitude (negative is West)	ggg.gggg
05	Speed over ground	Knots
06	GPS HDOP	-
07	Gyro Heading	Degrees (azimuth)
08	Course made good	Degrees (azimuth)
09	Mast PAR	$\mu\text{Einsteins/meter}^2 \text{ sec}$
10	Sea surface temperature	$^{\circ}\text{C}$
11	Sea surface conductivity	siemens/meter
12	Sea surface salinity	PSU
13	Sea depth (uncorrected, calc. sw sound vel. 1500 m/s)	meters
14	True wind speed (max speed windbird)	meters/sec
15	True wind direction (max speed windbird)	degrees (azimuth)
16	Ambient air temperature	$^{\circ}\text{C}$
17	Relative humidity	%
18	Barometric pressure	mBars
19	Sea surface fluorometry	volts (0-5 FSO)
20	Not used	-
21	PSP	$\text{W/m}^2$
22	PIR	$\text{W/m}^2$

## MGD77

The MGD77 data set is contained in a single file for the entire cruise. It can be found in the top level of the distribution data structure as NBP0808.mgd. The file NBP0808.gmt is created from the MGD77 dataset using the “mgd77togmt” utility. NBP0808.gmt can be used with the GMT plotting package.

The data used to produce the NBP0808.mgd file can be found on the distribution media in the file /process/0808proc.tar. The data files in the archive contain a day’s data and follow the naming convention Dddd.fnl.gz, where ddd is the year-day. These files follow a space-delimited columnar format that may be more accessible for some purposes. They contain data at one-second intervals rather than one minute and are individually “gzipped” to save space. Below is a detailed description of the MGD77 data set format. The other files in the archive contain interim processing files and are included to simplify possible reprocessing of the data using the RVDAS NBP processing scripts.

All decimal points are implied. Leading zeros and blanks are equivalent. Unknown or unused fields are filled with 9’s. All “corrections”, such as time zone, diurnal magnetics, and EOTVOS, are understood to be added.

Col	Len	Type	Contents	Description, Possible Values, Notes
1	1	Int	Data record type	Set to “5” for data record
2-9	8	Char	Survey identifier	
10-12	3	int	Time zone correction	Corrects time (in characters 13-27) to GMT when added; 0 = GMT
13-16	4	int	Year	4 digit year
17-18	2	int	Month	2 digit month
19-20	2	int	Day	2 digit day
21-22	2	int	Hour	2 digit hour
23-27	5	real	Minutes x 1000	
28-35	8	real	Latitude x 100000	+ = North - = South. (–9000000 to 9000000)
36-44	9	real	Longitude x 100000	+ = East - = West. (–18000000 to 18000000)
45	1	int	Position type code	1=Observed fix 3=Interpolated 9=Unspecified
46-51	6	real	Bathymetry, 2- way travel time	In 10,000th of seconds. Corrected for transducer depth and other such corrections
52-57	6	real	Bathymetry, corrected depth	In tenths of meters.
58-59	2	int	Bathymetric correction code	This code details the procedure used for determining the sound velocity correction to depth
60	1	int	Bathymetric type code	1 = Observed 3 = Interpolated (Header Seq. 12) 9 = Unspecified
61-66	6	real	Magnetics total field, 1 <sup>ST</sup> sensor	In tenths of nanoteslas (gammas)
67-72	6	real	Magnetics total field, 2 <sup>ND</sup> sensor	In tenths of nanoteslas (gammas), for trailing sensor
73-78	6	real	Magnetics residual field	In tenths of nanoteslas (gammas). The reference field used is in Header Seq. 13
79	1	int	Sensor for residual	1 = 1 <sup>st</sup> or leading sensor

Col	Len	Type	Contents	Description, Possible Values, Notes
			field	2 = 2 <sup>nd</sup> or trailing sensor 9 = Unspecified
80-84	5	real	Magnetics diurnal correction	In tenths of nanoteslas (gammas). (In nanoteslas) if 9-filled (i.e., set to "+9999"), total and residual fields are assumed to be uncorrected; if used, total and residuals are assumed to have been already corrected.
85-90	6	F6.0	Depth or altitude of magnetics sensor	(In meters) + = Below sea level 3 = Above sea level
91-97	7	real	Observed gravity	In 10 <sup>th</sup> of mgals. Corrected for Eotvos, drift, tares
98-103	6	real	EOTVOS correction	In 10 <sup>th</sup> of mgals. $E = 7.5 V \cos \phi \sin \alpha + 0.0042 V^*V$
104-108	5	real	Free-air anomaly	In 10 <sup>th</sup> of mgals G = observed G = theoretical
109-113	5	char	Seismic line number	Cross-reference for seismic data
114-119	6	char	Seismic shot-point number	
120	1	int	Quality code for navigation	5= Suspected, by the originating institution 6= Suspected, by the data center 9= No identifiable problem found

## Science of Opportunity

### ADCP

The shipboard ADCP system measures currents in a depth range from about 30 to 300 m -- in good weather. In bad weather or in ice, the range is reduced, and sometimes no valid measurements are made. ADCP data collection is the OPP-funded project of Eric Firing (University of Hawaii) and Teri Chereskin (Scripps Institution of Oceanography). Data is collected on both the LMG and the NBP for the benefit of scientists on individual cruises, and for the long-term goal of building a profile of current structure in the Southern Ocean.

A data feed is sent from the ADCP system to RVDAS whenever a reference layer is acquired. This feed contains east and north vectors for ship's speed, relative to the reference layer, and ship's heading. Collected files (one per day) are archived in 0808adcp.tar in the directory /rvdas/nav.

### pCO<sub>2</sub>

The NBP carries a pCO<sub>2</sub> measurement system from Lamont-Doherty Earth Observatory (LDEO). pCO<sub>2</sub> data is recorded by RVDAS and transmitted to LDEO at the end of each cruise. You will find pCO<sub>2</sub> data in a file named 0808pco2.tar in the /process directory, which contains the pCO<sub>2</sub> instrument's data merged with GPS, meteorological and other oceanographic measurements. For more information contact Colm Sweeney (csweeney@ldeo.columbia.edu).

## Cruise Science

### ***CTD***

The ctd data has been placed in the tar file /ocean/0808ctd.tar. The archive contains tar files 0808proc.tar.

### **RVDAS**

The Research Vessel Data Acquisition System (RVDAS) was developed at Lamont-Doherty Earth Observatory of Columbia University and has been in use on its research ship for many years. It has been extensively adapted for use on the USAP research vessels.

Daily data processing of the RVDAS data is performed to calibrate and convert values into useable units and as a quality-control on operation of the DAS. Raw and processed data sets from RVDAS are included in the data distribution. The tables below provide detailed information on the sensors and data. Be sure to read the “Significant Acquisition Events” section for important information about data acquisition during this cruise.

### ***Sensors and Instruments***

RVDAS data is divided into two general categories, *underway and navigation*. They can be found on the distribution media as subdirectories under the top level rvdas directory: /rvdas/uw, and /rvdas/nav. Processed oceanographic data is in the top level directory, /process. Each instrument or sensor produces a data file named with its channel ID. Each data file is g-zipped to save space on the distribution media. Not all data types are collected every day or on every cruise.

The naming convention for data files produced by the sensors and instruments is

NBP[CruiseID][ChannelID].dDDD

Example:     NBP0808.met1.d126

- The CruiseID is the numeric name of the cruise, in this case, NBP0808.
- The ChannelID is a 4-character code representing the system being logged. An example is “met1,” the designation for meteorology.
- DDD is the day of year the data was collected

## Underway Sensors

### Meteorology and Radiometry

Measurement	Channel ID	Collect. Status	Rate	Instrument
Air Temperature	met1	continuous	1 sec	R.M. Young 41372LC
Relative Humidity	met1	continuous	1 sec	
Wind Speed/Direction	met1	continuous	1 sec	R.M. Young 05106
Barometer	met1	continuous	1 sec	R.M. Young 61201
PIR (LW radiation)	eng1	continuous	1 sec	Eppley PIR
PSP (SW radiation)	met1	continuous	1 sec	Eppley PSP
PAR	met1	continuous	1 sec	BSI QSR-240
GUV	pguv	continuous	2 sec	BSI PUV-2511
PUV	pguv	not collected		BSI PUG-2500

### Geophysics

Measurement	Channel ID	Collect. Status	Rate	Instrument
Gravimeter	grv1	continuous	10 sec*	LaCoste & Romberg
Magnetometer	mag1	not collected	15 sec	EG&G G-866
Bathymetry	bat1	not collected	Varies	ODEC Bathy 2000
Bathymetry	knu1	continuous	Varies	Knudsen 320B/R
Bathymetry	sim1	not collected	Varies	Simrad EK500 Sonar

\*Data is output every second but it only changes every 10 seconds.

### Oceanography

Measurement	Channel ID	Collect. Status	Rate	Instrument
Conductivity	tsg1	Continuous	6 sec	SeaBird SBE-21
Salinity	tsg1	Continuous	6 sec	Calc. from pri. temp
Sea Surface Temp	tsg1	Continuous	6 sec	SeaBird 3-01/S
Fluorometry	flr1	Continuous	1 sec	Turner 10-AU-005
Transmissometry	hdas	Continuous	6 sec	WET Lab C-Star
pCO <sub>2</sub>	pco2	Continuous	70 sec	(LDEO)
ADCP	adcp	Continuous	varies	RD Instruments



## **Navigational Instruments**

Measurement	Channel ID	Collect. Status	Rate	Instrument
Trimble GPS	PCOD	Continuous	1 sec	Trimble 20636-00SM
Gyro	gyr1	Continuous	0.2 sec	Yokogawa Gyro
SeaPath	seap	Continuous	1 sec	SeaPath 200

## ***Data***

Data is received from the RVDAS system via RS-232 serial connections. A time tag is added at the beginning of each line of data in the form,

```
yy+dd:hh:mm:ss.sss [data stream from instrument]
```

where

yy       = two-digit year  
ddd      = day of year  
hh       = 2 digit hour of the day  
mm       = 2 digit minute  
ss.sss   = seconds

All times are reported in UTC.

The delimiters that separate fields in the raw data files are often spaces and commas but can be other characters such as : = @. Occasionally no delimiter is present. Care should be taken when reprocessing the data that the field's separations are clearly understood.

In the sections below a sample data string is shown, followed by a table that lists the data contained in the string.

## Underway Data

Each section below describes a type of data file (file name extension in parentheses) followed by a typical line of data in the file. In the table(s) for each section is a description of the fields within each line of data. Note: most data files listed below will be included with each cruise's data distribution, however some types of files may be omitted if the instrument was not operating during the cruise. The available data files can be found in the /rvdas/uw directory on the distribution disc.

### Sound Velocity Probe (svp1)

00+348:01:59:52.128 1539.40

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

### Meteorology (met1)

01+322:00:03:27.306 04.5 292 010 05.7 294 010 0959.6 000.2 093.1

-000.1537 0001.0886 0012.8248

Field	Data	Units
1	RVDAS time tag	
2	Port anemometer speed (relative)	m/s
3	Port anemometer direction (relative)	deg
4	Port anemometer standard deviation	deg
5	Starboard anemometer speed (relative)	m/s
6	Starboard anemometer direction (relative)	deg
7	Starboard anemometer standard deviation	deg
8	Barometer	mBar
9	Air temperature	°C
10	Relative humidity	%
11	PSP (short wave radiation)*	mV
12	PIR (long wave radiation)*	mV
13	PAR (photosynthetically available radiation)*	mV

\*See page 21 for calculations.

### Knudsen (knud)

99+099:00:18:19.775 HF,305.2,LF,304.3

Field	Data	Units
1	RVDAS time tag	
2	HF = High frequency flag (12 kHz)	
3	High frequency depth	meters
4	LF = Low frequency flag (3.5 kHz)	
5	Low frequency depth	meters

**Thermosalinograph (tsg1)**

00+019:23:59:46.976 15A16CFC163F8C2C100

Field	Data	Units
1	RVDAS time tag	
2	Seabird hex string (see page 24 for conversion to real units)	

**Fluorometer (flr1)**

00+019:23:59:58.061 0 0818 :: 1/19/00 17:23:17 = 0.983 (RAW) 1.2 (C)

Field	Data	Units
1	RVDAS time tag	
2	Marker 0 to 8	
3	4-digit index	
4	Date	mm/dd/yy
5	Time	hh:mm:ss
6	Signal	
7	Signal units of measurement	
8	Cell temperature (if temperature compensation package is installed)	
9	Temperature units (if temperature compensation package is installed)	

**pCO<sub>2</sub> (pco2)**00+021:23:59:43.190 2000021.99920 2382.4 984.2 30.73 50.8 345.9 334.1 -1.70  
-68.046 -144.446 Equil

Field	Data	Units
1	RVDAS time tag	
2	pCO <sub>2</sub> time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temperature	°C
5	Barometer	MBar
6	Concentration	ppm
7	Equilibrated temperature	°C
8	pCO <sub>2</sub> pressure	microAtm
9	Flow rate	ml / min
10	Source ID #	1 or 2 digits
11	Valve position	1 or 2 digits
12	Flow source (Equil = pCO <sub>2</sub> measurement)	text

**Engineering (eng1)**

07+280:06:45:29.359 12.2655 16.29123 134.663 98.51914 83.71822 -  
3.354797 45.38742 -0.149594 15.25094 15.08044 NAN

Field	Data	Units
1	RVDAS time tag	
2	Power Supply Voltage	
3	Internal Case Temperature	
4	Pump #1 flow rate	L/min
5	Pump #2 flow rate	L/min
6	Seismic air pressure	Lbs/sq-in
7	PIR case resistance	Kohm
8	PIR case ratiometric output	mV
9	Freezer #1 temperature	C
10	Freezer #2 temperature	C
11	Freezer #3 temperature	C

\*See page 25 for PIR calculations.

**Hydro-DAS (hdas)**

07+280:00:00:19.352 12.16678 15.94557 244.7432 4432.954 61.5 66.5 80.5  
63

Field	Data	Units
1	RVDAS time tag	
2	Supply voltage	
3	Panel temperature	
4	Fluorometer	mV
5	Transmissometer	mV
6	Flow meter 1 frequency	Hz
7	Flow meter 2 frequency	Hz
8	Flow meter 3 frequency	Hz
9	Flow meter 4 frequency	Hz

**Micro-TSG (mtsg)**

07+280:00:00:48.058 -1.5017, 2.70111, 33.9692, 1440.723

Field	Data	Units
1	RVDAS time tag	
2	Temperature	C
3	Conductivity	s/m
4	Sound velocity	m/s

**GUV Data (pguv)**

07+288:00:00:45.399 101507 000049 .000226 1.627E0 5.253E0 5.831E-1  
4.382E-2 6.811E0 1.479E-2 6.719E0 45.707 17.954

Field	Data	Units
1	RVDAS time tag	
2	Date	mmddyy
3	Time (UTC)	hhmmss
4	Ed0Gnd	V
5	Ed0320	uW (cm <sup>2</sup> nm)
6	Ed0340	uW (cm <sup>2</sup> nm)
7	Ed0313	uW (cm <sup>2</sup> nm)
8	Ed0305	uW (cm <sup>2</sup> nm)
9	Ed0380	uW (cm <sup>2</sup> nm)
10	Ed0PAR	uE (cm <sup>2</sup> nm)
11	Ed0395	uW (cm <sup>2</sup> nm)

**Remote Temperature (rtmp)**

07+272:00:00:15.960 -1.7870

Field	Data	Units
1	RVDAS time tag	
2	Temperature at seawater intake	C

**Ultrasonic Anemometer (wind)**

07+271:00:09:34.240 \_A,139,007.55,M,+330.77,-001.52,65,\_01

Field	Data	Units
1	RVDAS time tag	
2	Code (unit identification)	
3	Wind direction	Degrees
4	Wind speed	m/s
5	Wind speed units (M=M/S)	
6	Sound speed	m/s
7	Temperature (sonic)	C
8	Status (0 = OK, 60 = OK and heated, other code = error state)	
9	Checksum	

## Navigational Data

### Seapath GPS (seap)

The Seapath GPS outputs the following data strings, four in NMEA format and two in proprietary PSXN format:

- GPZDA
- GPGGA
- GPVTG
- GPHDT
- [PSXN, 20](#)
- PSXN, 22
- PSXN, 23

#### GPZDA

02+253:00:00:00.772 \$GPZDA,235947.70,09,09,2002,,\*7F

Field	Data	Units
1	RVDAS time tag	
2	\$GPZDA	
3	time	hhmmss.ss
4	Day	dd
5	Month	mm
6	Year	yyyy
7	(empty field)	
8	Checksum	

#### GPGGA

02+253:00:00:00.938

GPGGA,235947.70,6629.239059,S,06827.668899,W,1,07,1.0,11.81,M,,M,,\*6F

Field	Data	Units
1	RVDAS time tag	
2	\$GPGGA	
3	time	hhmmss.ss
4	Latitude	ddmm.mmmmmm
5	N or S for north or south latitude	
6	Longitude	ddmm.mmmmmm
7	E or W for east or west longitude	
8	GPS quality indicator, 0=invalid, 1=GPS SPS, 2=DGPS, 3=PPS, 4=RTK, 5=float RTK, 6=dead reckoning	
9	number of satellites in use (00-99)	
10	HDOP	x.x
9	height above ellipsoid in meters	m.mm
11	M	
12	(empty field)	
13	M	
14	age of DGPS corrections in seconds	s.s
15	DGPS reference station ID (0000-1023)	
16	Checksum	



## GPVTG

02+253:00:00:00.940 \$INVTG,19.96,T,,M,4.9,N,,K,A\*39

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	course over ground, degrees true	d.dd
4	T	
5	,	
6	M	
7	speed over ground in knots	k.k
8	N	
9	,	
10	K	
11	Mode	
12	Checksum	

## GPHDT

02+253:00:00:00.941 \$GPHDT,20.62,T\*23

Field	Data	Units
1	RVDAS time tag	
2	\$GPHDT	
3	Heading, degrees true	d.dd
4	T	
5	Checksum	

## PSXN,20

02+253:00:00:00.942 \$PSXN,20,0.43,0.43\*39

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	20	
4	Horizontal position & velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
5	Height & vertical velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
6	Heading quality: 0=normal, 1=reduced performance, 2=invalid data	
7	Roll & pitch quality: 0=normal, 1=reduced performance, 2=invalid data	
8	Checksum	

## PSXN,22

02+253:00:00:00.942 \$PSXN,22,0.43,0.43\*39

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	22	
4	gyro calibration value since system start-up in degrees	d.dd
5	short term gyro offset in degrees	d.dd
6	Checksum	





**PSXN,23**

02+253:00:00:02.933 \$PSXN,23,0.47,0.57,20.62,0.03\*0C

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	23	
4	roll in degrees, positive with port side up	d.dd
5	pitch in degrees, positive with bow up	d.dd
6	Heading, degrees true	d.dd
7	heave in meters, positive down	m.mm
8	Checksum	

**Trimble (P-Code) GPS (PCOD)**

The Trimble GPS, which formerly output Precise Position (*P-Code*) strings, but now only outputs Standard Position (*Civilian*) strings, outputs three NMEA standard data strings:

- Position fix (GGA)
- Latitude / longitude (GLL),
- Track and ground speed (VTG)

**GGA: GPS Position Fix – Geoid/Ellipsoid**

01+319:00:04:11.193 \$GPGGA,000410.312,6227.8068,S,06043.6738,W,1,06,1.0,031.9,M,-017.4,M,,\*49

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGGA	
3	UTC time at position	hhmmss.sss
4	Latitude	ddmm.mmm
5	North (N) or South (S)	
6	Longitude	ddmm.mmm
7	East (E) or West (W)	
8	GPS quality: 0 = Fix not available or invalid 1 = GPS, SPS mode, fix valid 2 = DGPS (differential GPS), SPS mode, fix valid 3 = P-CODE PPS mode, fix valid	
9	Number of GPS satellites used	
10	HDOP (horizontal dilution of precision)	
11	Antenna height	meters
12	M for meters	
13	Geoidal height	meters
14	M for meters	
15	Age of differential GPS data (no data in the sample string)	
16	Differential reference station ID (no data in the sample string)	
17	Checksum (no delimiter before this field)	



**GLL: GPS Latitude/Longitude**

01+319:00:04:11.272 \$GPGLL,6227.8068,S,06043.6738,W,000410.312,A\*32

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGLL	
3	Latitude	degrees
4	North or South	
5	Longitude	degrees
6	East or West	
7	UTC of position	hhmmss.sss
8	Status of data (A = valid)	
9	Checksum	

**VTG: GPS Track and Ground Speed**

01+319:00:04:11.273 \$GPVTG,138.8,T,126.0,M,000.0,N,000.0,K\*49

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	Heading	degrees
4	Degrees true (T)	
5	Heading	degrees
6	Degrees magnetic (M)	
7	Ship speed	knots
8	N = knots	
9	Speed	km/hr
10	K = km per hour	
11	Checksum	

**Gyro Compass (gyr1)**

00+019:23:59:59.952 \$HEHDT 25034,-020\*73

Field	Data	Units
1	RVDAS time tag	
2	\$HEHDT	
3	Heading, Degrees True	degrees
5	Checksum	

**Sound Velocity Probe (svp1)**

00+348:01:59:52.128 1539.40

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

## ADCP Course (adcp)

00+019:23:59:59.099 \$PUHAW,UVH,-1.48,-0.51,250.6

Field	Data	Units
1	RVDAS time tag	
2	\$PUHAW	
3	UVH (E-W, N-S, Heading)	
4	Ship Speed relative to reference layer, east vector	knots
5	Ship Speed relative to reference layer, north vector	knots
6	Ship heading	degrees

## Processed Data

The processed data sets can be found in the /process directory and subdirectories. Note: many of the subdirectories contain intermediate datasets to facilitate further processing and are not intended to be end-products. Only the final product files and datasets are described below.

## pCO2-merged

00+346:23:58:20.672 2000346.9991 2398.4 1008.4 0.01 45.4 350.3 342.6 15.77

Equil -43.6826 173.1997 15.51 33.90 0.33 5.28 9.05 1007.57 40.0 14.87 182.44

Field	Data	Units
1	RVDAS time tag	
2	pCO <sub>2</sub> time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temperature	°C
5	Barometer	MBar
6	Concentration	ppm
7	Equilibrated temperature	°C
8	pCO <sub>2</sub> pressure	microAtm
9	Flow rate	ml / min
10	Source ID #	1 or 2 digits
11	Valve position	1 or 2 digits
12	Flow source (Equil = pCO <sub>2</sub> measurement)	text
13	RVDAS latitude	degrees
14	RVDAS longitude	degrees
15	TSG external temperature	°C
16	TSG salinity	PSU
17	TSG fluorometry	V
18	RVDAS true wind speed	m/s
19	RVDAS true wind direction	degrees
20	Barometric Pressure	mBars
21	Uncontaminated seawater pump flow rate	l/min
22	Speed over ground	knots
23	Course made good	degrees

**tsgfl**

00+075:00:00:04.467 -01.488 -01.720 02.6783 33.63748 1.002442 0.002442

Field	Data	Units
1	RVDAS time tag	
2	Internal water temperature	°C
3	Sea Surface Temperature	°C
4	Conductivity	μSiemens
5	Salinity	PSU
6	Fluorometry	V
7	Transmissivity	V

## Calculations

The file `instcoef.txt` located in the / directory contains the calibration factors for shipboard instruments. This was the file used by the RVDAS processing software.

### TSG

Raw TSG data is stored as a 20 byte (character) long hex string. Example:

00+019:23:59:46.976 15A16CFC163F8C2C100

Bytes	Data
1-4	Sensor Temperature (in wet lab)
5-8	Conductivity
9-14	Remote Temperature (near seawater intake)
15-18	Transmissometer voltage

The coefficients for temperature and conductivity sensors can be found the `instcoef.txt` file and on the calibrations sheets in the appendix.

#### Calculating Temperature – ITS-90

T = decimal equivalent of bytes 1-4  
 Temperature Frequency:  $f = T/19 + 2100$   
 $\text{Temperature} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15$  (°C)

#### Calculating Conductivity – ITS-90

C = decimal equivalent of bytes 5-8  
 Conductivity Frequency  $f = \sqrt{C*2100+6250000}$   
 $\text{Conductivity} = (g + hf^2 + if^3 + jf^4)/[10(1 + \delta t + \epsilon p)]$  (siemens/meter)  
 t = temperature (°C); p = pressure (decibars);  $\delta = Ct_{cor}$ ;  $\epsilon = CP_{cor}$

#### Calculating Transmittance

$V_{dark} = 0.058$  V  
 $V_{ref} = 4.765$  V  
 t = decimal equivalent of bytes 18 - 20  
 Transmissometer Voltage ( $V_{signal}$ ) = t/819  
 $\% \text{ Transmittance} = (V_{signal} - V_{dark}) / (V_{ref} - V_{dark})$

### PAR

raw data = mV  
 calibration scale =  $6.27 \text{ V}/(\mu\text{Einstiens}/\text{cm}^2\text{sec})$   
 offset ( $V_{dark}$ ) = 0.1 mV  
 $(\text{raw mV} - V_{dark})/\text{scale} \times 104 \text{ cm}^2/\text{m}^2 \times 10^{-3} \text{ V/mV} = \mu\text{Einstiens}/\text{m}^2\text{sec}$   
 or  
 $(\text{data mV} - 0.1 \text{ mV}) \times 1.65 (\mu\text{Einstiens}/\text{m}^2\text{sec})/\text{mV} = \mu\text{Einstiens}/\text{m}^2\text{sec}$

## PSP

```
raw data = mV
calibration scale = 7.92 x 10-6 V/(W/m2)
data mV / (scale x 103 mV/V) = W/m2
or
data mV x 120.7 (W/m2)/V = W/m2
```

## PIR

Coefficient `pirCoeff` for this cruise can be found in the `instcoef.txt` file. Variable `PIRr` is the PIR case resistance and `PIRmv` is the radiometric output, as described in the “eng1” file description. Hard-coded “C” coefficients are shown below:

```
C1=0.0010295
C2=0.0002391
C3=0.0000001568
C4=5.6704e-8
```

Calculations (extracted from the C code):

```
raw data = mV
calibration scale = 4.16 x 10-6 V/(W/m2)
data mV / (scale x 103 mV/V) = W/m2
or
data mV x 120.7 (W/m2)/V = W/m2
Rr = log(fabs(PIRr * 1000))
T = 1 / ( C1 + (C2 * Rr) + (C3 * Rr * Rr * Rr) )
Rin = ( (PIRmv * 1000) / pirCoeff) + (C4 * T * T * T * T )
```



## Acquisition Problems and Events

This section lists problems with acquisition noted during this cruise including instrument failures, data acquisition system failures and any other factor affecting this data set. The format is ddd:hh:mm (ddd is year-day, hh is hour, and mm is minute). Times are reported in GMT.

Start	End	Description
193:03:12		Started Loggers.
193:17:45		RVDAS wasn't logging to disk. Killed and restarted.
195:00:47		Exited Argentinean EEZ.
198		Rebooted DAS.
201:02:28		Changed sound velocity on Knudsen from 1500m/s to 1400m/s.
203:18:28		Found Knudsen not logging to disk. Turned it back on.
214:09:54		Entered Argentinean EEZ.
216:22:02		Ended data collection for NBP0808.

## Appendix: Sensors and Calibrations

### NBP0808 Shipboard Sensors:

<i>Sensor</i>	<i>Serial Number</i>	<i>Last Calibration Date</i>	<i>Comments</i>
<b>Meteorology &amp; Radiometers</b>			
Stbd Anemometer (Gill Ultrasonic)	071739	5/15/2007	Installed 7/19/2007
Port Anemometer	WM 46263	6/30/2007	Installed 7/19/2007
Stbd Anemometer	WM 73682	6/30/2007	Installed 7/19/2007
Bridge Anemometer	WM 45835	2/28/2007	Bridge (center)
Barometer	01705	12/1/2006	Installed 5/26/2008
Humidity/Wet Temp	06134	9/26/2006	Installed 5/26/2008
PIR	33023F3	6/20/2008	Installed 7/9/2008
PSP	33090F3	6/11/2008	Installed 7/9/2008
Mast PAR	6356	8/8/2007	Installed 8/28/2007
GUV (Mast)	25110203113	3/18/2008	Installed 4/18/2008
<b>Underway</b>			
TSG	2131020-3198	5/20/2006	Installed 02/7/2007
TSG Remote Temp (Primary)	3846730-0352	6/6/2007	Installed 7/15/2007
TSG Remote Temp (Secondary)	031267	4/12/2006	Installed 1/29/2007, Moved 6/10/2007
Micro TSG	4549120-0226	1/12/2008	Installed 6/1/2008
Fluorometer (Primary)	5333-FRXX	Un-calibrated	Installed 4/14/04
Fluorometer (Secondary)	AFL-044	5/31/2006	Installed 6/23/2007
Transmissometer	CST-557DR	12/20/2006	Installed 3/14/08

***NBP0808 CTD Sensors:***

Sensor	Serial Number	Last Calibration Date	Comments
CTD Fish	094857-0232	9/26/2006	
CTD Fish Pressure	43528	9/26/2006	
CTD Deck Unit	11P47914-0768	n/a	
Primary Temperature Sensor	03P2186	1/10/2008	
Secondary Temperature Sensor	03P2308	1/10/2008	
Primary Conductivity Sensor	041852	1/26/2008	
Secondary Conductivity Sensor	041850	6/26/2007	Noticed drift after cast 006 replaced with sensor 041314
Secondary Conductivity Sensor	041314		Starting with cast 007
Dissolved Oxygen Sensor (Primary)	0082	1/9/2008	
Dissolved Oxygen Sensor (Secondary)	0080	7/25/2007	
Fluorometer	AFL-016D	10/16/2006	Needed as spare for next cruise
Transmissometer	CST-889DR	7/27/2007	
CTD Pump (Primary)	051626	4/17/2008	In House Cal
CTD Pump (Secondary)	051646	4/17/2008	In House Cal
Altimeter	497	n/a	
Slip Ring Assembly	n/a	n/a	
Carousel Water Sampler	3211265-0066	n/a	

**Calibrations**

The following pages are replicas of current calibration sheets for the sensors used during this cruise.

### ***Gravity Tie Start (Punta Arenas)***

[illegible]

## Meteorology System

### Anemometer (Port)

#### RM Young Anemometer Calibration, Model 05106

S/N: 46263

Date: 30-Jun-07

Cal'd By: George Aukon

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.10	-0.10	0.0
200	0.98	0.90	0.08	1.9
500	2.45	2.30	0.15	4.8
1000	4.90	4.80	0.10	9.5
1500	7.35	7.30	0.05	14.3
2000	9.80	9.80	0.00	19.0
3000	14.70	14.70	0.00	28.6
4000	19.60	19.60	0.00	38.1
5000	24.50	24.60	-0.10	47.6
6000	29.40	29.40	0.00	57.1
7000	34.30	34.30	0.00	66.6
8000	39.20	39.40	-0.20	76.2
9000	44.10	44.20	-0.10	85.7
10000	49.00	49.10	-0.10	95.2
12000	58.80	58.90	-0.10	114.2

Direction	Measured Direction	Delta Direction
0	0	0
30	30	0
60	59	1
90	89	1
120	118	2
150	148	2
180	179	1
210	210	0
240	240	0
270	270	0
300	300	0
330	330	0
0	0	0

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.10	-0.10
200	0.98	0.80	0.18
500	2.45	2.40	0.05
1000	4.90	4.80	0.10
1500	7.35	7.30	0.05
2000	9.80	9.80	0.00
3000	14.70	14.70	0.00
4000	19.60	19.60	0.00
5000	24.50	24.60	-0.10
6000	29.40	29.50	-0.10
7000	34.30	34.40	-0.10
8000	39.20	39.30	-0.10
9000	44.10	44.30	-0.20
10000	49.00	49.20	-0.20
12000	58.80	58.90	-0.10

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm?	2
Wind Direction Threshold < 30 gm?	15

Additional Comments

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

**Anemometer (Starboard)****RM Young Anemometer Calibration, Model 05106**

S/N: 73682

Date: 30-Jun-07

Cal'd By: George Aukon

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.10	-0.10	0.0
200	0.98	0.80	0.18	1.9
500	2.45	2.40	0.05	4.8
1000	4.90	4.80	0.10	9.5
1500	7.35	7.30	0.05	14.3
2000	9.80	9.80	0.00	19.0
3000	14.70	14.70	0.00	28.6
4000	19.60	19.60	0.00	38.1
5000	24.50	24.60	-0.10	47.6
6000	29.40	29.50	-0.10	57.1
7000	34.30	34.40	-0.10	66.6
8000	39.20	39.30	-0.10	76.2
9000	44.10	44.30	-0.20	85.7
10000	49.00	49.20	-0.20	95.2
12000	58.80	58.90	-0.10	114.2

Direction	Measured Direction	Delta Direction
0	0	0
30	29	1
60	59	1
90	89	1
120	119	1
150	148	2
180	178	2
210	207	3
240	237	3
270	267	3
300	297	3
330	328	2
0	0	0

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.10	-0.10
200	0.98	0.90	0.08
500	2.45	2.30	0.15
1000	4.90	4.80	0.10
1500	7.35	7.30	0.05
2000	9.80	9.80	0.00
3000	14.70	14.70	0.00
4000	19.60	19.60	0.00
5000	24.50	24.60	-0.10
6000	29.40	29.40	0.00
7000	34.30	34.30	0.00
8000	39.20	39.40	-0.20
9000	44.10	44.20	-0.10
10000	49.00	49.10	-0.10
12000	58.80	58.90	-0.10

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm? 2.3  
Wind Direction Threshold < 30 gm? 15

Additional Comments

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

**Anemometer (Bridge)****RM Young Anemometer Calibration, Model 05106**

S/N: 45835

Date: 28-Feb-07

Cal'd By: George Aukon

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.00	0.00	0.0
200	0.98	0.90	0.08	1.9
500	2.45	2.40	0.05	4.8
1000	4.90	4.80	0.10	9.5
1500	7.35	7.30	0.05	14.3
2000	9.80	9.80	0.00	19.0
3000	14.70	14.60	0.10	28.6
4000	19.60	19.50	0.10	38.1
5000	24.50	24.30	0.20	47.6
6000	29.40	29.20	0.20	57.1
7000	34.30	34.10	0.20	66.6
8000	39.20	39.00	0.20	76.2
9000	44.10	43.90	0.20	85.7
10000	49.00	48.80	0.20	95.2
12000	58.80	58.60	0.20	114.2

Direction	Measured Direction	Delta Direction
0	359	0
30	29	1
60	59	1
90	89	1
120	119	1
150	148	2
180	179	1
210	210	0
240	240	0
270	270	0
300	301	-1
330	331	-1
0	1	-1

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.00	0.00
200	0.98	1.00	-0.02
500	2.45	2.50	-0.05
1000	4.90	4.90	0.00
1500	7.35	7.40	-0.05
2000	9.80	9.80	0.00
3000	14.70	14.80	-0.10
4000	19.60	19.80	-0.20
5000	24.50	24.60	-0.10
6000	29.40	29.50	-0.10
7000	34.30	34.50	-0.20
8000	39.20	39.40	-0.20
9000	44.10	44.40	-0.30
10000	49.00	49.30	-0.30
12000	58.80	59.60	-0.80

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm? ☒ yes  
 Wind Direction Threshold < 30 gm? ☒ yes

**Additional Comments**

Potentiometer and potentiometer coupling were replaced, vertical shaft bearings were cleaned and lubricated.

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

**Barometer**

**R.M. Young Company**  
2801 Aero Park Drive  
Traverse City, Michigan 49686 USA

**Barometric Pressure Sensor Calibration Report**

Customer: *Raytheon Technical Services Co*

Test Number: 60621

Customer PO: RM31245-50

Test Date: 1 December 2006

Sales Order: 8800

**Test Sensor:**

Model: 61201

Serial Number: BP01705

Description: Barometric Pressure Sensor

Report of calibration comparison of test barometric pressure sensor with National Institute of Standards and Technology traceable standard pressure calibrator at five pressures in the R.M. Young Company controlled pressure facility. Calibration accuracy  $\pm 1.0$  hPa.

Reference Pressure (hPa)	Voltage Output (millivolts)	Indicated (1) Pressure (hPa)
800.0	0	800.0
875.0	1251	875.1
950.0	2501	950.1
1025.0	3750	1025.0
1100.0	4998	1099.9

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

**Reference Instrument**

Druck Pressure Controller Model DPI515  
Fluke Multimeter Model 8060A

**Serial # NIST Test Reference**

51500497 UKAS Lab 0221  
4865407 234027

Tested By: *E. Chumney*

METEOROLOGICAL INSTRUMENTS

Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com



**Humidity Sensor**

R.M. Young Company  
2801 Aero Park Drive  
Traverse City, Michigan 49686 USA

3-0.4  
**COPY**

**Relative Humidity Sensor Calibration Report**

Customer: *Raytheon Technical Services Co LLC*

Test Number: 69292R  
Test Date: 29 September 2006

Customer PO: RM29548.50  
Sales Order: 8708

**Test Sensor:**

Model: 41372LC Serial Number: 6134  
Description: Temperature/Relative Humidity Sensor

Report of calibration comparison of test relative humidity sensor with National Institute of Standards and Technology traceable standard relative humidity sensor at five humidity levels in the R.M. Young Company controlled humidity chamber facility. Calibration accuracy  $\pm 2.0$  %.

Reference Humidity (%)	Current Output (milliamps)	Indicated (1) Humidity (%)
10.4	5.9	11.9
30.4	8.8	30.2
49.7	12.0	50.0
69.9	15.2	69.8
89.6	17.9	86.6

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

**Reference Instrument**

Vaisala Humidity Sensor Model 35AC  
Fluke Multimeter Model 8060A

**Serial # NIST Test Reference**

N475040 TN 266152  
4865407 234027

Tested By: *E. Channing*

*page 2*

METEOROLOGICAL INSTRUMENTS

Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com

**Temperature Sensor**

**R.M. Young Company**  
2801 Aero Park Drive  
Traverse City, Michigan 49686 USA

3-04  
met

**Temperature Sensor Calibration Report**

Customer: **Raytheon Technical Services Co LLC**

Test Number: 69292      Customer PO: RM29548-50  
Test Date: 29 September 2006      Sales Order: 8708

<b>Test Sensor:</b>	
Model: 41372LC	Serial Number: 6134
Description: Temperature/Relative Humidity Sensor	

Report of calibration comparison of test temperature sensor with National Institute of Standards and Technology traceable standard thermometers at three temperatures in the R.M. Young Company controlled temperature calibration bath facilities. Calibration accuracy  $\pm 0.1^\circ$  Celsius.

Bath Temperature (degrees C)	Current Output (milliamps)	Indicated (1) Temperature (degrees C)
-50.03	3.992	-50.05
0.03	12.003	0.02
50.03	20.004	50.03

(1) Calculated from current output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument	Serial #	NIST Test Reference
Brooklyn Thermometer Model 43-FC	8006-118	204365
Brooklyn Thermometer Model 22332-D5-FC	25071	249763
Brooklyn Thermometer Model 2X400-D7-FC	77532	228060
Keithley Multimeter Model 191	15232	234027

Tested By:

*EChen*

page 1

METEOROLOGICAL INSTRUMENTS

Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com

**PIR****THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA

Telephone: 401-847-1020

Fax: 401-847-1031

Email: info@eppleylab.com

Internet: www.eppleylab.com



Scientific Instruments  
for Precision Measurements  
Since 1917

## STANDARDIZATION OF EPPLEY PRECISION INFRARED RADIOMETER Model PIR

Serial Number: 33023F3

Resistance: 739  $\Omega$  at 23  $^{\circ}\text{C}$   
Temperature Compensation Range:  $-20^{\circ}$  to  $+40^{\circ}$   $^{\circ}\text{C}$

This pyrgeometer has been compared against Eppley's Blackbody Calibration System under radiation intensities of approximately 200 watts meter<sup>-2</sup> and an average ambient temperature of 25  $^{\circ}\text{C}$  as measured by Standard Omega Temperature Probe, RTD#1.

As a result of a series of comparisons, it has been found to have a sensitivity of:

3.90  $\times 10^{-6}$  volts/watts meter<sup>-2</sup>

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 700 watts meter<sup>-2</sup>. This radiometer is linear to within  $\pm 1.0\%$  up to this intensity.

The calibration of this instrument is traceable to the International Practical Temperature Scale (IPTS) through a precision low-temperature blackbody.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".

Shipped to: Raytheon Technical Services Date of Test: June 13, 2008  
National Science Foundation  
Port Hueneme, CA

S.O. Number: 61667  
Date: June 20, 2008

In Charge of Test:

Reviewed by:

Remarks:

**PSP****THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA

Telephone: 401-847-1020

Fax: 401-847-1031

Email: info@eppleylab.com

Internet: www.eppleylab.com

Scientific Instruments  
for Precision Measurements  
Since 1917**STANDARDIZATION OF  
EPPLEY PRECISION SPECTRAL PYRANOMETER  
Model PSP**

Serial Number: 33090F3

Resistance: 700  $\Omega$  at 23  $^{\circ}\text{C}$ Temperature Compensation Range:  $-20^{\circ}$  to  $+40^{\circ}\text{C}$ 

This radiometer has been compared with Standard Precision Spectral Pyranometer, Serial Number 21231F3 in Eppley's Integrating Hemisphere under radiation intensities of approximately 700 watts meter<sup>-2</sup> (roughly one half a solar constant).

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$8.06 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 1400 watts meter<sup>-2</sup>. This radiometer is linear to within  $\pm 0.5\%$  up to this intensity.

The calibration of this instrument is traceable to standard self-calibrating cavity pyrhemometers in terms of the Systems Internationale des Unites (SI units), which participated in the Tenth International Pyrheliometric Comparisons (IPC X) at Davos, Switzerland in September-October 2005.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".


Useful conversion facts: 1 cal cm<sup>-2</sup> min<sup>-1</sup> = 697.3 watts meter<sup>-2</sup>  
1 BTU/ft<sup>2</sup>-hr<sup>-1</sup> = 3.153 watts meter<sup>-2</sup>

Shipped to: Raytheon Technical Services Date of Test: June 11, 2008  
National Science Foundation  
Port Hueneme, CA

In Charge of Test: 

S.O. Number: 61666

Date: June 20, 2008

Reviewed by: 

Remarks:

**PAR****Biospherical Instruments Inc.****CALIBRATION CERTIFICATE**

Calibration Date 8/8/2007  
 Model Number QSR-240  
 Serial Number 6356  
 Operator TPC  
 Standard Lamp HEC-1630(10/25/2006)  
 Probe Excitation Voltage Range: 6 to 18 VDC(+)  
 Output Polarity: Positive

Probe Conditions at Calibration(In air):

Calibration Voltage: 6 VDC(+)  
 Probe Current: 1.2 mA

Probe Output Voltage:

Probe Illuminated 93.1 mV  
 Probe Dark -0.1 mV  
 Probe Net Response 93.1 mV  
 RG780 Filter 0.1 mV

Corrected Lamp Output:

Output In Air (same condition as calibration):

9.56E+15 quanta/cm<sup>2</sup>sec  
0.01588 uE/cm<sup>2</sup>sec

Calibration Scale Factor:

(To calculate irradiance, divide the net voltage reading in Volts by this value.)

Dry: 9.7383E-18 V/(quanta/cm<sup>2</sup>sec)  
5.8644E+00 V/(uE/cm<sup>2</sup>sec)

Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with alcohol.
4. Calibration was performed with customer cable, when available.

QSR240R 05/24/95



**GUV**

Biospherical Instruments Inc.

GUV-2511 Calibration Certificate										
System Serial Number		25110203113			Date of Calibration		3/18/08			
Calibration database		25110203113v4.mdb			Date of Certificate		3/18/2008			
DASSN		0068			Standard of Spectral Irradiance		91537(10/25/06)			
Microprocessor Tag Number		2			Operator		TC			
Monochromatic Channels		Wavelength [nm]	Responsivity [Amps per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	ScaleSmall [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	ScaleMedium [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	ScaleLarge [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
Ed0320		2	2.7010E-10	2.7551E-05	8.0491E-03	2.8497E+00	6.5000E-05	6.4000E-05	2.2300E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0340		6	2.2027E-10	2.2467E-05	6.5640E-03	2.3144E+00	3.7400E-04	3.7600E-04	1.1590E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0313		8	2.4100E-10	2.4539E-05	7.1692E-03	2.5594E+00	1.0000E-04	1.0000E-04	6.9100E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0305		10	1.6600E-11	1.6943E-06	4.9499E-04	1.5313E-01	4.1300E-04	4.0500E-04	-2.2080E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0380		12	7.0759E-11	7.2174E-06	2.1086E-03	7.0320E-01	1.1140E-03	1.1050E-03	-1.4780E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0395		18	3.4926E-10	3.5624E-05	1.0408E-02	3.3997E+00	1.3100E-04	1.3000E-04	2.2300E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Broadband Channels		Wavelength [nm]	Responsivity [Amps per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	ScaleSmall [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	ScaleMedium [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	ScaleLarge [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
Ed0PAR		13	1.9205E-05	1.9589E+00	5.7230E+02	2.0376E+05	8.8600E-04	8.7700E-04	-1.3030E-03	$\mu\text{E}/(\text{cm}^2\cdot\text{sec})$
Auxiliary Channels		Wavelength [nm]	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement Units
Ed0Gnd		0	1	1	1	1	0	0	0	V
Ed0Temp		22	1	0.01	0.01	0.01	0	0	0	C
Ed0Vin		27	1	-0.25	-0.25	-0.25	0	0	0	V

© Biospherical Instruments Inc., 5340 Riley Street, San Diego, California 92110 USA. Contact [support@biospherical.com](mailto:support@biospherical.com) for more information.

## TSG Calibration Files

## Underway Conductivity

## SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 3198  
 CALIBRATION DATE: 20-May-06

SBE21 CONDUCTIVITY CALIBRATION DATA  
 PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## GHIJ COEFFICIENTS

g = -4.27061383e+000  
 h = 5.04384737e-001  
 i = -4.53257393e-004  
 j = 4.72934991e-005  
 CPcor = -9.5700e-008 (nominal)  
 CTcor = 3.2500e-006 (nominal)

## ABCDM COEFFICIENTS

a = 2.81077465e-006  
 b = 5.02715558e-001  
 c = -4.26259709e+000  
 d = -8.83813520e-005  
 m = 4.8  
 CPcor = -9.5700e-008 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2.91246	0.00000	0.00000
1.0000	34.8123	2.97566	8.21793	2.97567	0.00002
4.6261	34.7919	3.29397	8.59263	3.29396	-0.00001
15.0000	34.7503	4.26437	9.64425	4.26434	-0.00003
18.4999	34.7417	4.60953	9.99119	4.60955	0.00002
24.0000	34.7323	5.16751	10.52728	5.16752	0.00001
29.0000	34.7279	5.68947	11.00456	5.68948	0.00001
32.4999	34.7263	6.06206	11.33261	6.06205	-0.00001

Conductivity =  $(g + hf^2 + if^3 + jf^4) / [10(1 + \delta t + \epsilon p)]$  Siemens/meter

Conductivity =  $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$  Siemens/meter

t = temperature[°C]; p = pressure[decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

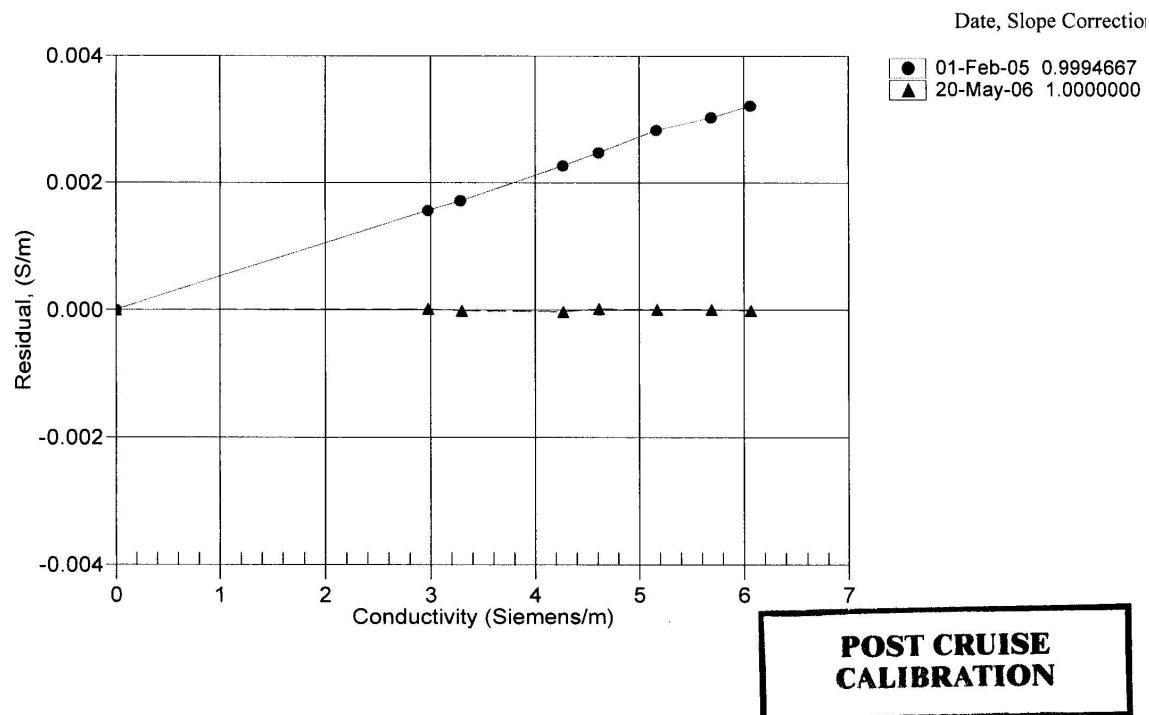

**Underway Temperature Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 3198  
CALIBRATION DATE: 20-May-06SBE21 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.22473160e-003$   
 $h = 6.29770835e-004$   
 $i = 2.05272425e-005$   
 $j = 1.54706370e-006$   
 $f0 = 1000.0$

## ITS-68 COEFFICIENTS


$a = 3.64763347e-003$   
 $b = 5.95315785e-004$   
 $c = 1.61762223e-005$   
 $d = 1.54852177e-006$   
 $f0 = 2568.439$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	2568.439	1.0001	0.00011
4.6261	2782.830	4.6259	-0.00021
15.0000	3467.526	15.0002	0.00020
18.4999	3723.433	18.5000	0.00006
24.0000	4152.193	23.9998	-0.00023
29.0000	4571.111	29.0000	0.00004
32.4999	4881.298	32.4999	0.00004

$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 * T_{90}$  (-2 to 35  $^\circ\text{C}$ )

Residual = instrument temperature - bath temperature

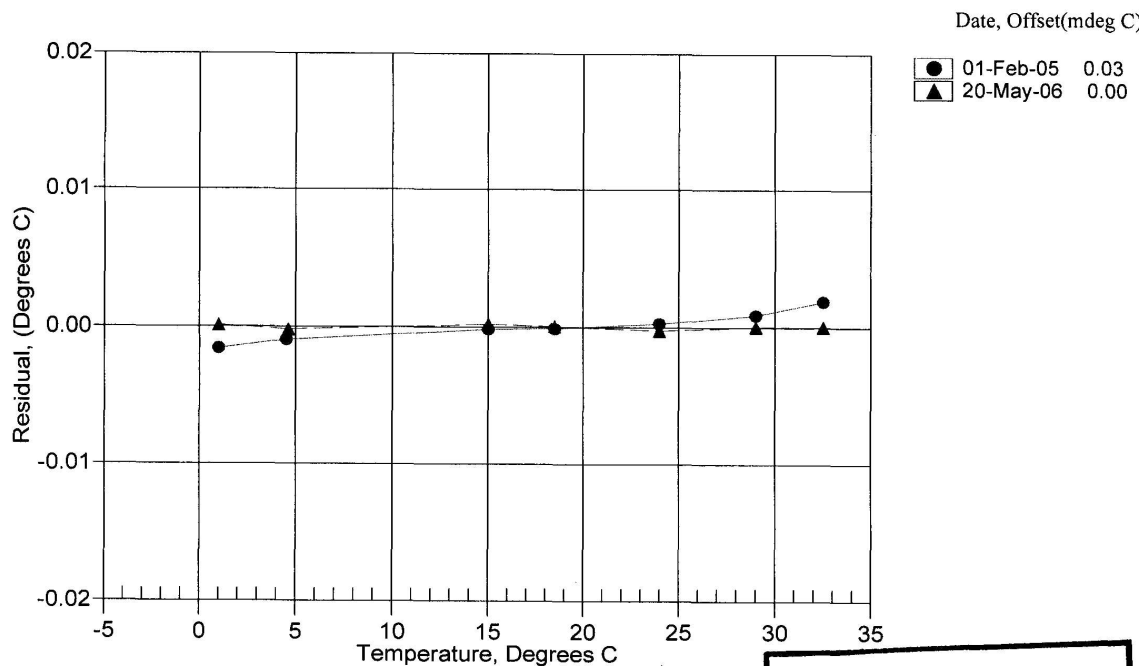
**POST CRUISE  
CALIBRATION**



**Underway Temperature Sensor (Primary Remote)**

44

**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0352  
CALIBRATION DATE: 06-Jun-07SBE 38 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE


## ITS-90 COEFFICIENTS

 $a_0 = -1.791146e-005$   
 $a_1 = 2.748666e-004$   
 $a_2 = -2.288718e-006$   
 $a_3 = 1.522128e-007$ 

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.50010	809858.1	-1.50005	0.00005
0.99990	723216.3	0.99986	+0.00004
4.50000	619038.5	4.49993	+0.00007
7.99990	531605.5	7.99989	+0.00001
11.50000	457969.9	11.50002	0.00002
14.99990	395755.0	15.00000	0.00010
18.49990	343018.4	18.49995	0.00005
22.00000	298175.3	21.99994	+0.00006
25.50000	259928.8	25.49995	+0.00005
29.00000	227212.0	28.99995	-0.00005
32.50000	199144.2	32.50006	0.00006

$$\text{Temperature ITS-90} = 1/(a_0 + a_1 \ln(n)) + a_2 [\ln(n)]^2 + a_3 [\ln(n)]^3 - 273.15 \text{ (}^\circ\text{C)}$$

Residual = instrument temperature - bath temperature

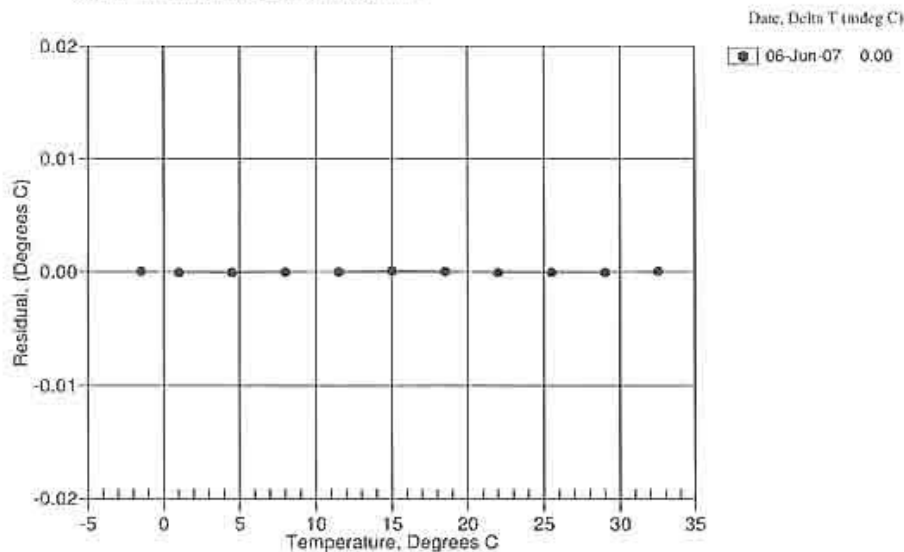

**Underway Temperature Sensor (Secondary Remote)****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1267  
CALIBRATION DATE: 12-Apr-06SBE3 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.76625066e-003$   
 $h = 6.64522185e-004$   
 $i = 2.84261863e-005$   
 $j = 2.62601374e-006$   
 $f_0 = 1000.0$

## ITS-68 COEFFICIENTS


$a = 3.68121498e-003$   
 $b = 5.89543636e-004$   
 $c = 1.47312260e-005$   
 $d = 2.62748536e-006$   
 $f_0 = 5707.029$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5001	5707.029	-1.5002	-0.00010
1.0000	6042.027	1.0001	0.00005
4.4999	6534.652	4.5000	0.00014
7.9999	7055.608	8.0000	0.00007
11.4999	7605.659	11.4998	-0.00008
14.9999	8185.578	14.9998	-0.00014
18.4999	8796.088	18.4998	-0.00011
22.0000	9437.895	22.0000	-0.00003
25.4999	10111.624	25.5001	0.00019
28.9999	10817.898	29.0001	0.00019
32.4999	11557.257	32.4997	-0.00019

$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 * T_{90}$  (-2 to 35  $^\circ\text{C}$ )

Residual = instrument temperature - bath temperature

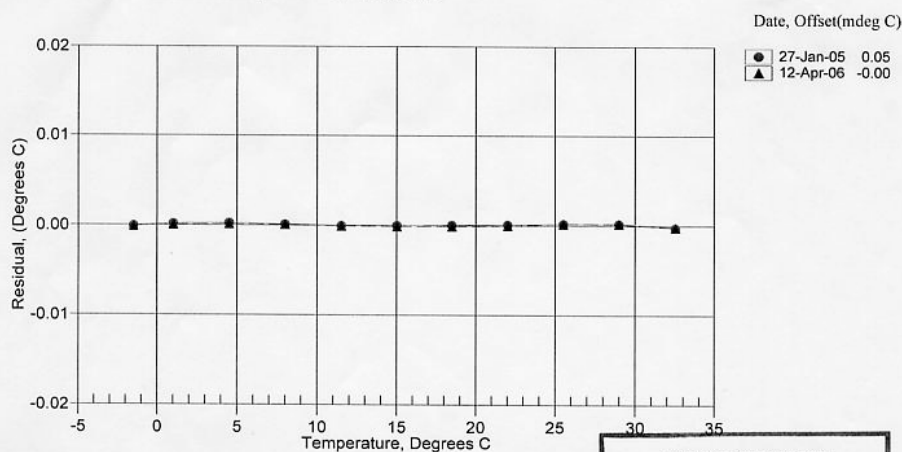**POST CRUISE  
CALIBRATION**

**Micro-TSG Calibration Files*****Temperature Sensor (Micro-TSG)***

Sensor Serial No: 0226

TCALDATE=12-Jan-08

TA0=-6.625307e-005

TA1= 2.870318e-004

TA2=-3.279891e-006

TA3= 1.750784e-007

Sea Bird Electronics, Inc  
1808 136<sup>th</sup> Place NE  
Bellevue, WA 98005

***Conductivity Sensor (Micro-TSG)***

Sensor Serial No: 0226

CCALDATE=12-Jan-08

CG=-1.014919e+000

CH= 1.569437e-001

CI=-4.469846e-004

CJ= 6.064779e-005

CTCOR= 3.250000e-006

CPCOR=-9.570000e-008

WBOTC= 9.807243e-007

Sea Bird Electronics, Inc  
1808 136<sup>th</sup> Place NE  
Bellevue, WA 98005

**Underway fluorometer (Primary)**

PO Box 518  
620 Applegate St.  
Philomath OR 97370



(541) 929-5650  
Fax (541) 929-5277  
<http://www.wetlabs.com>

**Chlorophyll Fluorometer Characterization**

**Date:** 05/31/06  
**Serial #:** AFL-044  
**Job#:** 0209007  
**Tech:** K.C

**Dark Counts** 0.177 volts  
**CEV** 2.725 volts  
**SF** 9.8116

**FSV** 5.45 volts

**Linearity:** 0.999 R<sup>2</sup> (0–1.5 volts)  
0.995 R<sup>2</sup> (0– 5.45 volts)

**Notes:**

**Dark Counts:** Signal output of the meter in clean water with black tape over detector.

**CEV** is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to **25 µg/l** of a *Thalassiosira weissflogii* phytoplankton culture.

**SF** is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determined by using the following equation:  
 $SF = (25) / (CEV - \text{dark})$  e.g.  $(25) / (2.865 - 0.238) = 9.516$

**FSV** is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m<sup>3</sup>) can be derived by using the following equation: (µg/l) = (V<sub>measured</sub> – CWO) \* SF

The relationship between fluorescence and chlorophyll-*a* concentrations in-situ is high variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [ Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

**Underway Transmissometer**

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 929-5650  
Fax (541) 929-5277  
[www.wetlabs.com](http://www.wetlabs.com)

**C-Star Calibration and Repairs**

Date	12/20/2006	Customer	Raytheon Polar Services
Job #	021020	S/N#	CST-557DR
		Work order	007

**Repairs and Modifications:**

Replaced bulkhead connector, 38 mm lens and o-rings. Baked to remove moisture. Recalibrated.

**Comments:**

- Shake-tested unit
- Pressure-tested unit
- Noise test: 1 sample/sec for 60 sec
- Stability test: 1 sample/min for 12 hrs
- Performed water calibration
- Temperature test, 27–2 °C
- Updated unit's calibration sheet

cstarwkbkf1.xls

Revision F

6/12/03

**CTD Pressure Sensor (fish)****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0232  
CALIBRATION DATE: 26-Sep-06SBE9plus PRESSURE CALIBRATION DATA  
10000 psia S/N 43528

## DIGIQUARTZ COEFFICIENTS:

C1 = -5.103000e+004  
 C2 = 8.606365e-002  
 C3 = 1.481220e-002  
 D1 = 3.642300e-002  
 D2 = 0.000000e+000  
 T1 = 3.004925e+001  
 T2 = -3.406308e-004  
 T3 = 4.125600e-006  
 T4 = 1.811600e-009  
 T5 = 0.000000e+000


## AD590M, AD590B, SLOPE AND OFFSET:

AD590M = 1.13600e-002  
 AD590B = -8.42350e+000  
 Slope = 0.99978  
 Offset = 0.0319 (dbars)

PRESSURE (PSIA)	INST OUTPUT(Hz)	INST TEMP(C)	INST OUTPUT (PSIA)	CORRECTED INST OUTPUT (PSIA)	RESIDUAL (PSIA)
14.675	33289.50	21.9	14.568	14.615	-0.060
2001.705	33930.70	22.1	2002.284	2001.886	0.181
3988.395	34558.00	22.1	3989.251	3988.409	0.014
5975.164	35172.50	22.2	5976.527	5975.241	0.077
7962.097	35774.80	22.2	7963.884	7962.154	0.057
9949.272	36365.50	22.3	9951.215	9949.041	-0.231
7961.761	35774.70	22.4	7963.436	7961.706	-0.055
5974.924	35172.50	22.5	5976.351	5975.065	0.141
3988.024	34558.00	22.5	3988.996	3988.154	0.130
2001.221	33930.60	22.6	2001.645	2001.247	0.026
14.671	33289.60	22.9	14.346	14.392	-0.279

Residual = corrected instrument pressure - reference pressure

Date, Avg Offset (psia)

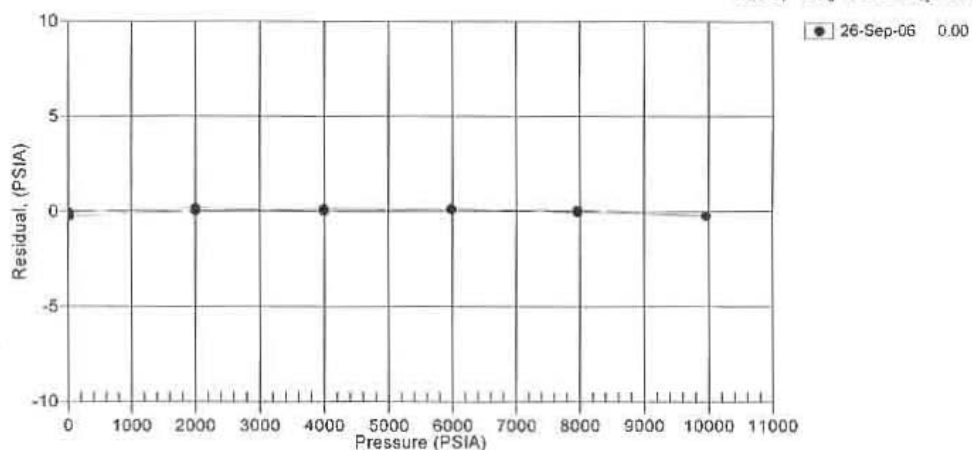

**CTD Primary Temperature Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2186  
CALIBRATION DATE: 10-Jan-08SBE3 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.34004885e-003$   
 $h = 6.44357902e-004$   
 $i = 2.30359279e-005$   
 $j = 2.14466833e-006$   
 $f0 = 1000.0$

## IPTS-68 COEFFICIENTS


$a = 3.68121353e-003$   
 $b = 6.02943002e-004$   
 $c = 1.62526134e-005$   
 $d = 2.14621884e-006$   
 $f0 = 2882.302$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5001	2882.302	-1.5001	0.00001
0.9999	3047.621	0.9999	-0.00001
4.4999	3290.441	4.4999	-0.00003
7.9999	3546.873	7.9999	0.00000
11.4999	3817.278	11.4999	0.00004
14.9999	4102.010	15.0000	0.00005
18.4999	4401.404	18.4999	-0.00005
21.9999	4715.808	21.9998	-0.00009
25.4999	5045.555	25.4999	0.00004
28.9999	5390.931	29.0000	0.00009
32.4999	5752.220	32.4999	-0.00005

$$\text{Temperature ITS-90} = 1/[g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]] - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature IPTS-68} = 1/[a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]] - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 * T_{90}$  (-2 to 35  $^\circ\text{C}$ )

Residual = instrument temperature - bath temperature

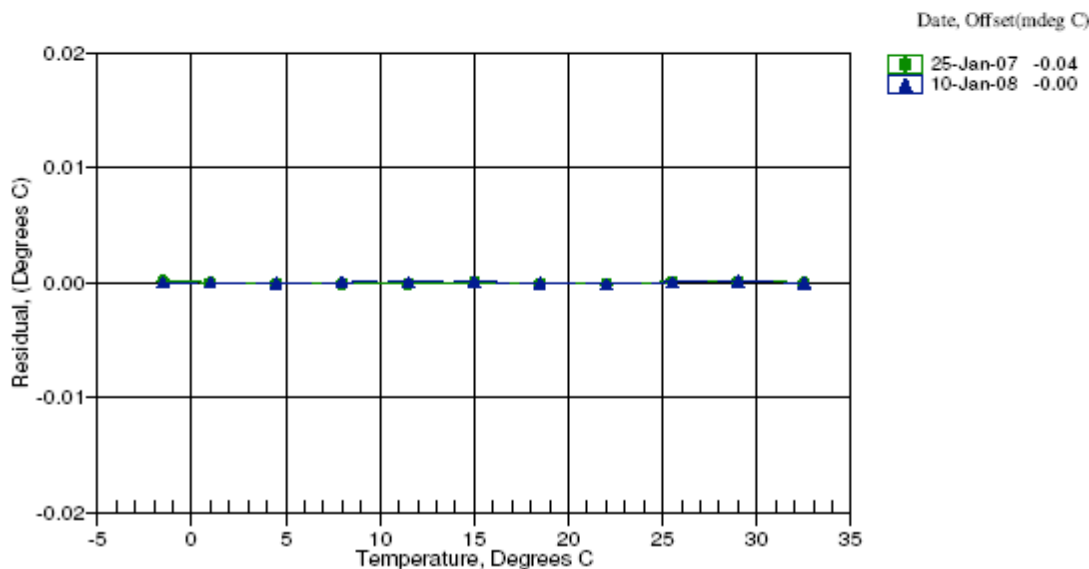

**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

**Temperature Calibration Report**

Customer:	Raytheon Polar Services Co.		
Job Number:	48653	Date of Report:	1/10/2008
Model Number:	SBE 03Plus	Serial Number:	03P2186

*Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.*

*An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.*

**'AS RECEIVED CALIBRATION'**☒ **Performed** ☐ **Not Performed**

Date: 1/10/2008

Drift since last cal: +0.00004 Degrees Celsius/year

Comments:

**'CALIBRATION AFTER REPAIR'**☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: Degrees Celsius/year

Comments:



**CTD Secondary Temperature Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2308  
CALIBRATION DATE: 10-Jan-08SBE3 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS

$g = 4.34505775e-003$   
 $h = 6.44550497e-004$   
 $i = 2.32217908e-005$   
 $j = 2.16913976e-006$   
 $f0 = 1000.0$

## IPTS-68 COEFFICIENTS


$a = 3.68121362e-003$   
 $b = 6.02554500e-004$   
 $c = 1.63069131e-005$   
 $d = 2.17069685e-006$   
 $f0 = 2906.243$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5001	2906.243	-1.5001	0.00000
0.9999	3073.048	0.9999	0.00000
4.4999	3318.063	4.4999	-0.00003
7.9999	3576.831	7.9999	0.00000
11.4999	3849.717	11.4999	0.00003
14.9999	4137.079	14.9999	0.00003
18.4999	4439.261	18.4999	-0.00004
21.9999	4756.612	21.9998	-0.00006
25.4999	5089.463	25.4999	0.00003
28.9999	5438.111	29.0000	0.00006
32.4999	5802.850	32.4999	-0.00003

$$\text{Temperature ITS-90} = 1 / \{ g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)] \} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature IPTS-68} = 1 / \{ a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)] \} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 * T_{90}$  (-2 to 35  $^\circ\text{C}$ )

Residual = instrument temperature - bath temperature

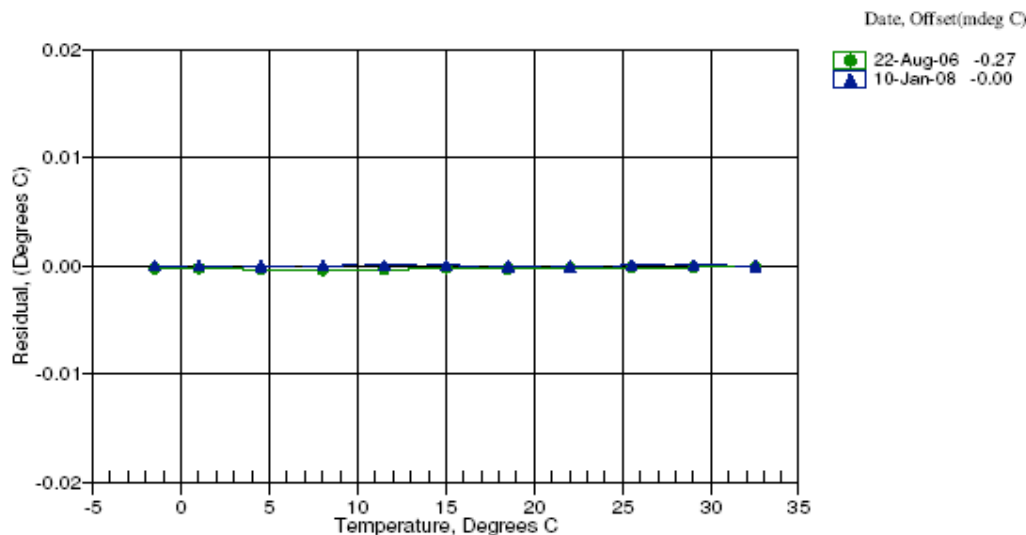

**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

**Temperature Calibration Report**

Customer:	Raytheon Polar Services Co.		
Job Number:	48653	Date of Report:	1/10/2008
Model Number:	SBE 03Plus	Serial Number:	03P2308

*Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.*

*An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.*

**'AS RECEIVED CALIBRATION'**☒ **Performed** ☐ **Not Performed**

Date: 1/10/2008

Drift since last cal: +0.00019 Degrees Celsius/year

Comments:

**'CALIBRATION AFTER REPAIR'**☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: Degrees Celsius/year

Comments:

**CTD Primary Conductivity Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1852  
CALIBRATION DATE: 10-Jan-08SBE4 CONDUCTIVITY CALIBRATION DATA  
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## GHJ COEFFICIENTS


$g = -3.96023791e+000$   
 $h = 5.05695912e-001$   
 $i = -5.54651278e-004$   
 $j = 5.41198276e-005$   
 $CP_{cor} = -9.5700e-008$  (nominal)  
 $CT_{cor} = 3.2500e-006$  (nominal)

## ABCDM COEFFICIENTS

$a = 1.34913219e-006$   
 $b = 5.03785467e-001$   
 $c = -3.95422179e+000$   
 $d = -8.58070150e-005$   
 $m = 5.1$   
 $CP_{cor} = -9.5700e-008$  (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.80157	0.00000	0.00000
-1.0000	34.9569	2.81484	7.97604	2.81484	0.00000
1.0000	34.9569	2.98683	8.18637	2.98684	0.00001
15.0000	34.9578	4.28713	9.62657	4.28709	-0.00004
18.5000	34.9569	4.63500	9.97607	4.63502	0.00002
29.0001	34.9510	5.72190	10.99480	5.72194	0.00004
32.5000	34.9401	6.09513	11.32281	6.09510	-0.00003

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / (10(1 + \delta t + \epsilon p)) \text{ Siemens/meter}$$
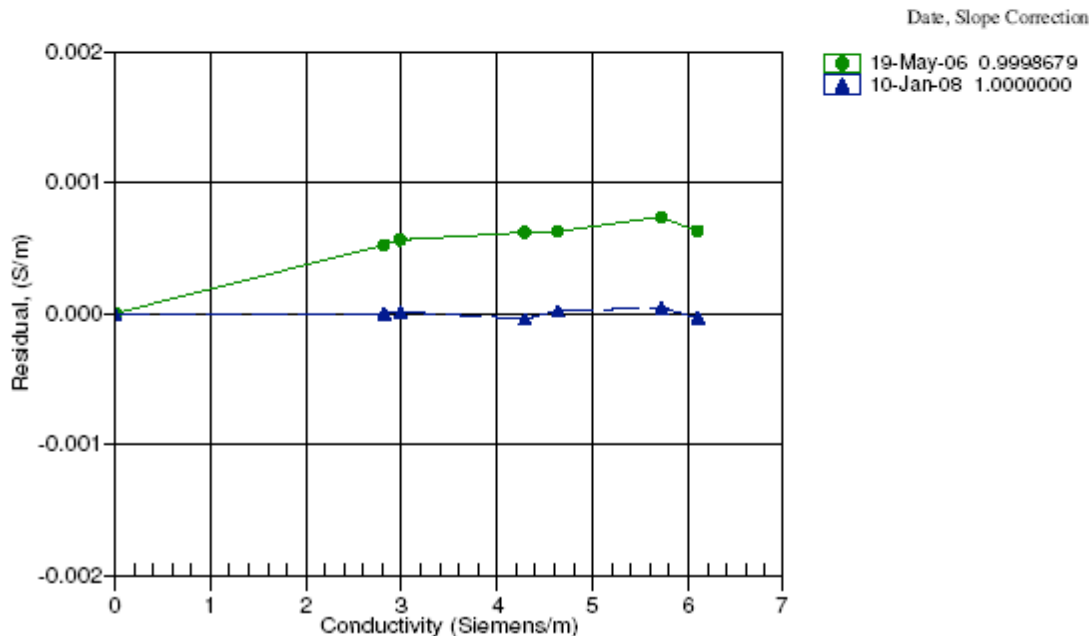
$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10(1 + \epsilon p)] \text{ Siemens/meter}$$
 $t = \text{temperature}[^{\circ}\text{C}]; p = \text{pressure[decibars]}; \delta = CT_{cor}; \epsilon = CP_{cor};$ 
 $\text{Residual} = (\text{instrument conductivity} - \text{bath conductivity}) \text{ using } g, h, i, j \text{ coefficients}$ 


**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

**Conductivity Calibration Report**

Customer:	Raytheon Polar Services Co.		
Job Number:	48654	Date of Report:	1/10/2008
Model Number:	SBE 04C	Serial Number:	041852

Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.

**'AS RECEIVED CALIBRATION'**☒ **Performed** ☐ **Not Performed**

Date: 1/10/2008

Drift since last cal: -0.00020 PSU/month\*

Comments:

**'CALIBRATION AFTER CLEANING & REPLATINIZING'**☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: PSU/month\*

Comments:

\*Measured at 3.0 S/m

Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.

## CTD Secondary Conductivity Senesor (cast 001 -006)

**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1850

CALIBRATION DATE: 26-Jun-07

SBE4 CONDUCTIVITY CALIBRATION DATA

PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

## GHJ COEFFICIENTS

g = -4.34346018e+000

h = 5.22284785e-001

i = 8.35673592e-005

j = 2.23102434e-005

CPcor = -9.5700e-008 (nominal)

CTcor = 3.2500e-006 (nominal)

## ABCDM COEFFICIENTS

a = 4.56237821e-005

b = 5.22463069e-001

c = -4.34399624e+000

d = -8.41199524e-005

m = 3.8

CPcor = -9.5700e-008 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.88261	0.00000	0.00000
-1.0002	34.9338	2.81314	7.86998	2.81315	0.00001
0.9999	34.9342	2.98507	8.07497	2.98510	0.00002
14.9999	34.9346	4.28458	9.48007	4.28445	-0.00013
18.4999	34.9334	4.63221	9.82165	4.63227	0.00005
28.9999	34.9290	5.71868	10.81828	5.71883	0.00014
32.4999	34.9217	6.09227	11.13976	6.09217	-0.00010

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / (10(1 + \delta t + \epsilon p)) \text{ Siemens/meter}$$

$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10(1 + \epsilon p)] \text{ Siemens/meter}$$
t = temperature[°C]; p = pressure[decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correcti

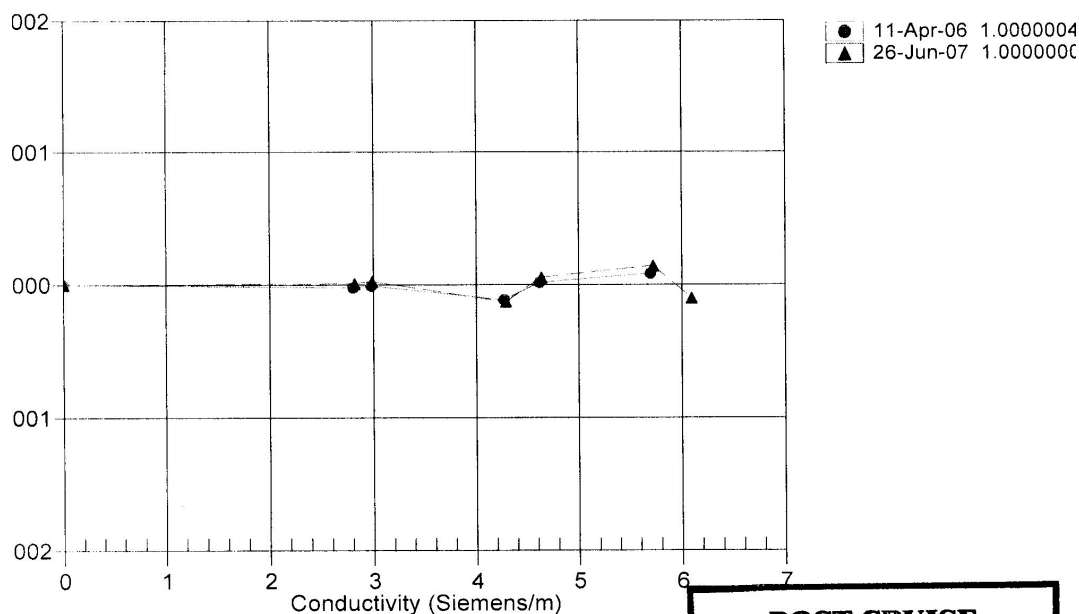
**POST CRUISE  
CALIBRATION**

**CTD Secondary Conductivity Senesor (cast 007 – on)**

**SEA-BIRD ELECTRONICS, INC.**  
 1808 136th Place N.E., Bellevue, Washington, 98005 USA  
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1314  
 CALIBRATION DATE: 08-Feb-08

SBE4 CONDUCTIVITY CALIBRATION DATA  
 PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

**GHIJ COEFFICIENTS**

g = -4.07432471e+000  
 h = 4.70852950e-001  
 i = -3.55317882e-005  
 j = 2.78698286e-005  
 CPcor = -9.5700e-008 (nominal)  
 CTcor = 3.2500e-006 (nominal)

**ABCDM COEFFICIENTS**

a = 2.57454097e-005  
 b = 4.70693911e-001  
 c = -4.07357148e+000  
 d = -7.95977201e-005  
 m = 4.0  
 CPcor = -9.5700e-008 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.94118	0.00000	0.00000
-1.0000	34.9363	2.81334	8.25650	2.81332	-0.00002
1.0000	34.9359	2.98521	8.47318	2.98524	0.00003
15.0000	34.9369	4.28484	9.95748	4.28482	-0.00002
18.5000	34.9367	4.63261	10.31787	4.63260	-0.00001
29.0001	34.9319	5.71913	11.36885	5.71917	0.00005
32.5000	34.9226	6.09242	11.70754	6.09239	-0.00003

Conductivity =  $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$  Siemens/meter

Conductivity =  $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$  Siemens/meter

t = temperature[°C]; p = pressure[decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

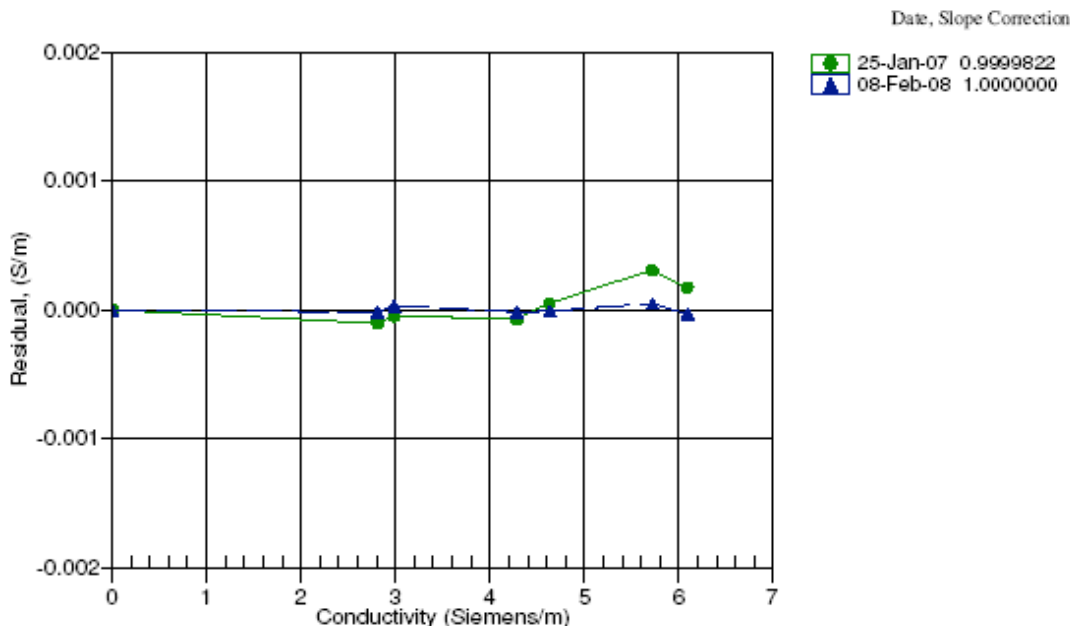

**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

**Conductivity Calibration Report**

Customer:	Raytheon Polar Services Co.		
Job Number:	49000	Date of Report:	2/8/2008
Model Number:	SBE 04-02/0	Serial Number:	041314

Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.

**'AS RECEIVED CALIBRATION'**☒ **Performed** ☐ **Not Performed**

Date: 2/8/2008

Drift since last cal: 0.0000 PSU/month\*

Comments:

**'CALIBRATION AFTER CLEANING & REPLATINIZING'**☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: PSU/month\*

Comments:

\*Measured at 3.0 S/m

Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.

**CTD Primary Dissolved Oxygen Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0082  
CALIBRATION DATE: 09-Jan-08p

## SBE43 OXYGEN CALIBRATION DATA

## COEFFICIENTS

Soc = 0.2920

Boc = 0.0000

Voffset = -0.6150

TCor = 0.0008


PCor = 1.350e-04

BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.23	20.00	0.01	1.271	1.24	0.01
1.24	26.00	0.01	1.347	1.24	0.00
1.24	12.00	0.01	1.176	1.25	0.01
1.24	2.00	0.00	1.053	1.24	-0.00
1.24	6.00	0.00	1.104	1.25	0.00
1.26	30.00	0.02	1.413	1.26	-0.00
4.09	20.00	0.01	2.792	4.11	0.01
4.11	26.00	0.01	3.041	4.10	-0.00
4.12	12.00	0.01	2.479	4.14	0.02
4.14	6.00	0.00	2.239	4.15	0.00
4.15	30.00	0.02	3.231	4.13	-0.01
4.16	2.00	0.00	2.078	4.14	-0.03
6.65	26.00	0.01	4.544	6.64	-0.01
6.67	30.00	0.02	4.830	6.66	-0.01
6.69	20.00	0.01	4.173	6.71	0.02
6.76	12.00	0.01	3.673	6.79	0.03
6.82	6.00	0.00	3.292	6.84	0.01
6.85	2.00	0.00	3.027	6.82	-0.03

$$\text{oxygen (ml/l)} = (\text{Soc} * (\text{V} + \text{Voffset})) * \exp(\text{TCor} * \text{T}) * \text{Oxsat}(\text{T}, \text{S}) * \exp(\text{PCor} * \text{P})$$

V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU]

Oxsat(T,S) = oxygen saturation [ml/l], P = pressure [dbar], Residual = instrument oxygen - bath oxygen

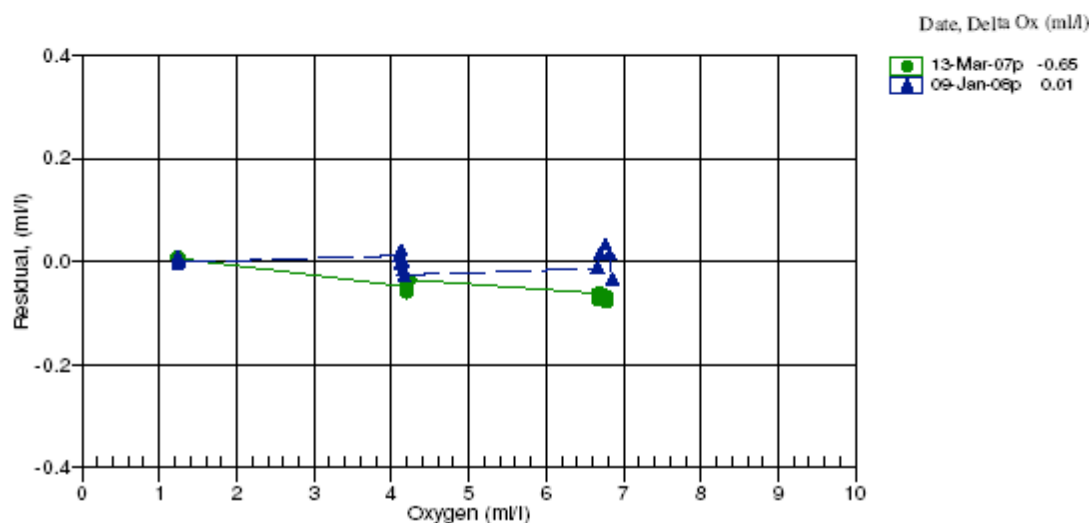



**CTD Secondary Dissolved Oxygen Sensor****SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0080  
CALIBRATION DATE: 25-Jul-07p**SBE 43 OXYGEN CALIBRATION DATA****COEFFICIENTS**

Soc = 0.3584

Boc = 0.0000

Voffset = -0.5056

TCor = 0.0018

PCor = 1.350e-04

BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.25	30.00	0.01	1.126	1.24	-0.01
1.25	20.00	0.01	1.050	1.28	0.03
1.25	26.00	0.01	1.098	1.26	0.01
1.25	2.00	0.00	0.862	1.24	-0.02
1.25	12.00	0.01	0.973	1.29	0.04
1.25	6.00	0.00	0.907	1.27	0.01
4.09	30.00	0.01	2.518	4.02	-0.07
4.10	20.00	0.01	2.276	4.18	0.07
4.11	26.00	0.01	2.436	4.10	-0.01
4.13	12.00	0.01	2.033	4.21	0.09
4.15	6.00	0.00	1.825	4.16	0.01
4.15	2.00	0.00	1.673	4.06	-0.09
6.47	30.00	0.01	3.692	6.36	-0.12
6.50	26.00	0.01	3.552	6.48	-0.02
6.54	20.00	0.01	3.324	6.65	0.11
6.62	6.00	0.00	2.609	6.63	0.01
6.62	12.00	0.01	2.955	6.76	0.14
6.64	2.00	0.00	2.373	6.49	-0.14


$$\text{oxygen (ml/l)} = (\text{Soc} * (\text{V} + \text{Voffset})) * \exp(\text{TCor} * \text{T}) * \text{Oxsat}(\text{T}, \text{S}) * \exp(\text{PCor} * \text{P})$$

V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU]

Oxsat(T,S) = oxygen saturation [ml/l], P = pressure [dbar]

Residual = instrument oxygen - bath oxygen

Date, Delta Ox (ml/l)

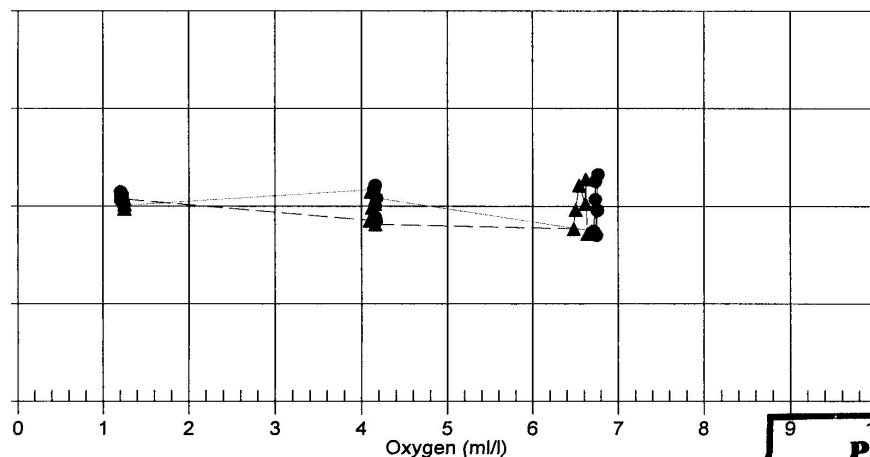

● 17-Aug-06p 0.37  
▲ 25-Jul-07p 0.03

**POST CRUISE  
CALIBRATION**

**CTD Fluorometer**

PO Box 518  
620 Applegate St.  
Philomath OR 97370



(541) 929-5650  
Fax (541) 929-5277  
<http://www.wetlabs.com>

**Chlorophyll Fluorometer Characterization**

**Date:** 10/16/06  
**Serial #:** AFL-016D  
**Job#:** 0102007  
**Tech:** K.C

**Dark Counts** 0.221 volts  
**CEV** 2.643 volts  
**SF** 10.3220

**FSV** 5.45 volts

**Linearity:** 0.999 R<sup>2</sup> (0–1.5 volts)  
0.995 R<sup>2</sup> (0– 5.45 volts)

**Notes:**

**Dark Counts:** Signal output of the meter in clean water with black tape over detector.

**CEV** is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to 25 µg/l of a *Thalassiosira weissflogii* phytoplankton culture.

**SF** is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determined by using the following equation:  
 $SF = (25) / (CEV - \text{dark})$  e.g.  $(25 / (2.865 - 0.238)) = 9.516$

**FSV** is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m<sup>3</sup>) can be derived by using the following equation: (µg/l) =  $(V_{\text{measured}} - \text{dark}) * SF$

The relationship between fluorescence and chlorophyll-*a* concentrations in-situ is highly variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [ Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

**CTD Transmissometer**

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 929-5650  
Fax (541) 929-5277  
[www.wetlabs.com](http://www.wetlabs.com)

**C-Star Calibration**

Date	July 27, 2007	Customer	National Science Foundation	Work order	002
Job #	0507014	S/N#	CST-889DR	Pathlength	25 cm

	Analog meter
$V_d$	0.060 V
$V_{air}$	4.837 V
$V_{ref}$	4.727 V

Temperature of calibration water	24.8 °C
Ambient temperature during calibration	26.1 °C

Relationship of transmittance ( $Tr$ ) to beam attenuation coefficient ( $c$ ), and pathlength ( $x$ ):  $Tr = e^{-cx}$

To determine beam transmittance:  $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient:  $c = -1/x * \ln(Tr)$

$V_d$  Meter output with the beam blocked. This is the offset.

$V_{air}$  Meter output in air with a clear beam path.

$V_{ref}$  Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain  $V_{ref}$ .

Ambient temperature: meter temperature in air during the calibration.

$V_{sig}$  Measured signal output of meter.

Revision G

3/5/07

