

Data Report NBP0806

Drake Passage

Dr. Ken Smith

May 31 – June 30, 2008



United States Antarctic Program

RVIB Nathaniel B. Palmer

Raytheon Polar Services

Prepared by Bill Jirsa and Paul Huckins

Table of Contents

INTRODUCTION	1
DISTRIBUTION CONTENTS AT A GLANCE	2
EXTRACTING DATA	3
DISTRIBUTION CONTENTS.....	4
CRUISE INFORMATION.....	4
<i>Cruise Track</i>	4
<i>Satellite Images</i>	4
NBP DATA PRODUCTS	4
<i>JGOFS</i>	4
<i>MGD77</i>	5
SCIENCE OF OPPORTUNITY	7
<i>ADCP</i>	7
<i>pCO₂</i>	7
CRUISE SCIENCE.....	7
<i>CTD</i>	7
<i>XBT</i>	7
<i>Mocness</i>	7
RVDAS.....	8
<i>Sensors and Instruments</i>	8
Underway Sensors	8
Meteorology and Radiometry.....	8
Geophysics	8
Oceanography.....	9
Navigational Instruments	9
<i>Data</i>	9
Underway Data	10
Sound Velocity Probe (svp1).....	10
Meteorology (met1).....	10
Gravimeter (grv1).....	10
Magnetometer (mag1)	11
Knudsen (knud)	12
Simrad EM120 (mbdp).....	12
Thermosalinograph (tsg1)	12
Fluorometer (flr1).....	12
pCO ₂ (pco2)	13
Engineering (eng1)	13
Hydro-DAS (hdas).....	13
Micro-TSG (mtsg).....	14
GUV Data (pguv)	14
Remote Temperature (rtmp).....	14
Ultrasonic Anemometer (wind).....	14
Navigational Data	16
Seapath GPS (seap)	16
Trimble (P-Code) GPS (PCOD)	18
Gyro Compass (gyr1)	19
ADCP Course (adcp).....	19
Sound Velocity Probe (svp1).....	20
Processed Data	20
pCO ₂ -merged	20
tsgfl	20
CALCULATIONS.....	22
TSG.....	22
PAR	22
PSP	23

PIR.....	23
ACQUISITION PROBLEMS AND EVENTS.....	24
APPENDIX: SENSORS AND CALIBRATIONS	25
NBP0806 Shipboard Sensors:	25
METEOROLOGY & RADIOMETERS	25
UNDERWAY	25
NBP0806 CTD Sensors:	25
NBP0806 MOCNESS Sensors:	26
Note:	26
CALIBRATIONS	26
Gravity Tie Start (Punta Arenas)	27
METEOROLOGY SYSTEM	28
Anemometer (Port)	28
Anemometer (Starboard)	29
Anemometer (Bridge)	30
Barometer	31
Humidity Sensor	32
Temperature Sensor.....	33
PIR.....	34
PSP	35
PAR.....	36
GUV.....	37
TSG CALIBRATION FILES.....	38
Underway Conductivity.....	38
Underway Temperature Sensor.....	39
Underway Temperature Sensor (Primary Remote).....	40
Underway Temperature Sensor (Secondary Remote)	41
MICRO-TSG CALIBRATION FILES	42
Temperature Sensor (Micro-TSG).....	42
Conductivity Sensor (Micro-TSG).....	42
Underway fluorometer (Primary).....	43
Underway Transmissometer.....	44
CTD Pressure Sensor (fish).....	45
CTD Primary Temperature Sensor	46
CTD Secondary Temperature Sensor.....	48
CTD Primary Conductivity Sensor.....	50
CTD Secondary Conductivity Senesor (cast 007 – on)	53
CTD Primary Dissolved Oxygen Sensor	55
CTD Secondary Dissolved Oxygen Sensor.....	56
CTD Fluorometer	57
CTD Transmissometer.....	58
MOCNESS	59
Mocness Temperature Sensor.....	59
Mocness Conductivity Sensor.....	60
Mocness Fluorometer Sensor	62
Mocness Transmissometer Sensor.....	64

Introduction

The NBP data acquisition systems continuously log data from the instruments used during the cruise. This document describes:

- The structure and organization of the data on the distribution media
- The format and contents of the data strings
- Formulas for calculating values
- Information about the specific instruments in use during the cruise
- A log of acquisition problems and events during the cruise that may affect the data
- Scanned calibration sheets for the instruments in use during the cruise.

The data is distributed on a DVD-R or CD-ROM written in ISO9660 level-1 format. It is readable by virtually every computing platform.

All the data has been compressed using Unix “gzip,” identified by the “.gz” extension. It has been copied to the distribution media in the Unix tar archive format, “.tar” extension. Tools are available on all platforms for uncompressing and de-archiving these formats: On Macintosh, use Stuffit Expander with DropStuff. On Windows operating systems use WinZip.

MultiBeam and BathyW data, if collected, are distributed separately.

IMPORTANT: Read the last section, “Acquisition Problems and Events,” for important information that may affect the processing of this data.

Distribution Contents at a Glance

Volume 1 of 1: NBP0806

File	Description
/	Root level directory
NBP0806.trk	Text file of cruise track (lat,lon)
NBP0806.mgd	Full Cruise MGD77 data file
NBP0806.gmt	GMT binary file of MGD77 data
INSTCOEF.TXT	Instrument Coefficient File
0806_trk.gif	Visual cruise track reference
Airplane.mov	MBARI RC plane Video
/process	Geop data
0806jgof.tar	JGOFS format data files
0806qc.tar	Daily RVDAS QC postscript plots
0806pco2.tar	Merged pCO2 data files
0806mgd.tar	MGD Data
0806proc.tar	Other processed data
/rvdas/nav	Navigation data
0806gyr1.tar	Gyro raw data
0806PCOD.tar	Trimble P-code raw data
0806seap.tar	Seapath data
0806adcp.tar	ADCP Data Sets
0806gp02	Gp02 Data
/rvdas/uw	Underway data
0806bwnc.tar	Baltic Winch raw data
0806swnc.tar	Starboard Winch raw data
0806uwnc.tar	Upper Waterfall Winch raw data
0806flr1.tar	Fluorometer raw data
0806grv1.tar	Gravimeter raw data
0806met1.tar	Meteorology raw data
0806oyo1.tar	Seismic acquisition data
0806pco2.tar	pCO2 raw data
0806wind.tar	Ultrasonic anemometer raw data
0806tsg1.tar	TSG raw data
0806svp1.tar	Sound velocity probe (in ADCP well)
0806syn1.tar	Syntron data
0806mtsg.tar	Micro TSG data
0806eng1.tar	Engineering Data and PIR
0806hdas.tar	HydroDAS raw data
0806pguv.tar	GUV raw data
0806rtmp.tar	Remote temperature data
0806mbdp.tar	SIMRAD multibeam sonar data
0806knud.tar	Knudsen raw data
0806mag1.tar	Magnetometer raw data
/Imagery	Other Data, Files and Pictures
0806Imag.tar	Satellite imagery
/ocean	
0806ctd.tar	Ctd data

	0806xbt.tar	Xbt data
/Nutrient	0806Nuts.tar	Nutrient Report
	0806OMN.tar	Nutrient Data
/Mocness	MOCNESS.TAR	Mocness data
/181_182	Data Set	Data set collected after passing through British EEZ.

Extracting Data

The Unix tar command has many options. It is often useful to know exactly how an archive was produced when expanding its contents. All archives were created using the command,

```
tar cvf archive_filename files_to_archive
```

To create a list of the files in the archive, use the Unix command,

```
tar tvf archive_filename > contents.list
```

where `contents.list` is the name of the file to create

To extract the files from the archive:

```
tar xvf archive_filename file(s)_to_extract
```

G-zipped files will have a “.gz” extension on the filename. These files can be decompressed after de-archiving, using the Unix command,

```
gunzip filename.gz
```

Distribution Contents

Cruise Information

NBP0806 Departed Punta Arenas, Chile on May 30, 2008. There were no major problems during the transit and no instruments changed. The weather and the seas were very cooperative for most of the cruise resulting in low ratio of weather related noise in the standard data. There were over the side operations including MOCNESS, CTD, XBT and Tucker trawls. Other non-ship standard science was done, that data is not described in this report. NBP0806 returned to Punta Arenas on June 30. We crossed through Argentine waters on our way to and from the science area of interest. We crossed into British waters near the Falklands' during our return to Punta Arenas. That data was deleted from all data sets. There is one full data distribution and a second distribution of Argentine only data. This disk has 2 data sets on it. The main data set is in the root directory. That data is all the data from the time we started collecting data until the time we entered the British EEZ outside the Falkland Islands. We then entered the Argentine EEZ and resumed data collection. Data collected after we re-entered the Argentine EEZ is in the directory /181_182 (for Julian days 181 and 182). The file formats and directory structure of the data in /181_182 follow the conventions used in the primary data set in the root directory.

Cruise Track

The distribution DVD includes a GMT cruise track file (NBP0806.trk). It contains the longitude and latitude at one-minute intervals extracted from the NBP0806.gmt file.

A PostScript cruise track file has been produced and placed in the / directory.

Satellite Images

Satellite Images received for this cruise can be found in the file called 0804Imag.tar Imagery collected and processed on the ship is in two further subdirectories, Ice and WX (weather). Files are named using the convention, ssss_fff_mmddyy_tttt_ww.gif where:

ssss_fff = satellite and flight number
 mm = month
 dd = day
 yy = year
 tttt = time in hours and minutes (UTC)
 ww = optional field for identifying wavelength, such as vis (visible) or IR (infrared)

NBP Data Products

Two datasets are created on each cruise: JGOFS and MGD77.

The data processing scripts used to produce JGOFS and MGD77 data sets create a lot of intermediate files. These files are included on the data distribution media in a file called 0806proc.TAR. They are included to make re-processing easier in the event of an error, but no extensive detail of the formats is included in this document. If you have any questions, please contact jtessel@usap.gov.

JGOFS

The JGOFS data set can be found on the distribution media in the file /process/0806JGOF.tar. The archive contains one file produced for each day named jgDDD.dat.gz, where DDD is the year-day the data was acquired. The ".gz" extension indicates that the individual files are compressed before archiving. Each daily file consists of 22 columnar fields in text format as described in the table below. The JGOFS data set is created from calibrated data decimated at

one-minute intervals. Several fields are derived measurements from more than a single raw input. For example, Course Made Good (CMG) and Speed Over Ground (SOG) are calculated from gyro and GPS inputs. Daily plots during the cruise are produced from the JGOFS data set. Note: Null, unused, or unknown fields are indicated as "NAN" as 9999 in the JGOFS data.

Field	Data	Units
01	GMT date	dd/mm/yy
02	GMT time	hh:mm:ss
03	NGL latitude (negative is South)	tt.tttt
04	NGL longitude (negative is West)	ggg.gggg
05	Speed over ground	Knots
06	GPS HDOP	-
07	Gyro Heading	Degrees (azimuth)
08	Course made good	Degrees (azimuth)
09	Mast PAR	$\mu\text{Einsteins/meter}^2 \text{ sec}$
10	Sea surface temperature	$^{\circ}\text{C}$
11	Sea surface conductivity	siemens/meter
12	Sea surface salinity	PSU
13	Sea depth (uncorrected, calc. sw sound vel. 1500 m/s)	meters
14	True wind speed (max speed windbird)	meters/sec
15	True wind direction (max speed windbird)	degrees (azimuth)
16	Ambient air temperature	$^{\circ}\text{C}$
17	Relative humidity	%
18	Barometric pressure	mBars
19	Sea surface fluorometry	volts (0-5 FSO)
20	Not used	-
21	PSP	W/m^2
22	PIR	W/m^2

MGD77

The MGD77 data set is contained in a single file for the entire cruise. It can be found in the top level of the distribution data structure as NBP0806.mgd. The file NBP0806.gmt is created from the MGD77 dataset using the "mgd77togmt" utility. NBP0806.gmt can be used with the GMT plotting package.

The data used to produce the NBP0806.mgd file can be found on the distribution media in the file /process/0806proc.tar. The data files in the archive contain a day's data and follow the naming convention Dddd.fnl.gz, where ddd is the year-day. These files follow a space-delimited columnar format that may be more accessible for some purposes. They contain data at one-second intervals rather than one minute and are individually "gzipped" to save space. Below is a detailed description of the MGD77 data set format. The other files in the archive contain interim processing files and are included to simplify possible reprocessing of the data using the RVDAS NBP processing scripts.

All decimal points are implied. Leading zeros and blanks are equivalent. Unknown or unused fields are filled with 9's. All "corrections", such as time zone, diurnal magnetics, and EOTVOS, are understood to be added.

Col	Len	Type	Contents	Description, Possible Values, Notes
1	1	Int	Data record type	Set to "5" for data record
2-9	8	Char	Survey identifier	
10-12	3	int	Time zone correction	Corrects time (in characters 13-27) to GMT when added; 0 = GMT
13-16	4	int	Year	4 digit year
17-18	2	int	Month	2 digit month

Col	Len	Type	Contents	Description, Possible Values, Notes
19-20	2	int	Day	2 digit day
21-22	2	int	Hour	2 digit hour
23-27	5	real	Minutes x 1000	
28-35	8	real	Latitude x 100000	+ = North - = South. (–9000000 to 9000000)
36-44	9	real	Longitude x 100000	+ = East - = West. (–18000000 to 18000000)
45	1	int	Position type code	1=Observed fix 3=Interpolated 9=Unspecified
46-51	6	real	Bathymetry, 2- way travel time	In 10,000th of seconds. Corrected for transducer depth and other such corrections
52-57	6	real	Bathymetry, corrected depth	In tenths of meters.
58-59	2	int	Bathymetric correction code	This code details the procedure used for determining the sound velocity correction to depth
60	1	int	Bathymetric type code	1 = Observed 3 = Interpolated (Header Seq. 12) 9 = Unspecified
61-66	6	real	Magnetics total field, 1 ST sensor	In tenths of nanoteslas (gammas)
67-72	6	real	Magnetics total field, 2 ND sensor	In tenths of nanoteslas (gammas), for trailing sensor
73-78	6	real	Magnetics residual field	In tenths of nanoteslas (gammas). The reference field used is in Header Seq. 13
79	1	int	Sensor for residual field	1 = 1 st or leading sensor 2 = 2 nd or trailing sensor 9 = Unspecified
80-84	5	real	Magnetics diurnal correction	In tenths of nanoteslas (gammas). (In nanoteslas) if 9-filled (i.e., set to “+9999”), total and residual fields are assumed to be uncorrected; if used, total and residuals are assumed to have been already corrected.
85-90	6	F6.0	Depth or altitude of magnetics sensor	(In meters) + = Below sea level 3 = Above sea level
91-97	7	real	Observed gravity	In 10 th of mgals. Corrected for Eotvos, drift, tares
98-103	6	real	EOTVOS correction	In 10 th of mgals. $E = 7.5 V \cos \phi \sin \alpha + 0.0042 V * V$
104-108	5	real	Free-air anomaly	In 10 th of mgals G = observed G = theoretical
109-113	5	char	Seismic line number	Cross-reference for seismic data
114-119	6	char	Seismic shot-point number	
120	1	int	Quality code for navigation	5=Suspected, by the originating institution 6=Suspected, by the data center 9=No identifiable problem found

Science of Opportunity

ADCP

The shipboard ADCP system measures currents in a depth range from about 30 to 300 m -- in good weather. In bad weather or in ice, the range is reduced, and sometimes no valid measurements are made. ADCP data collection is the OPP-funded project of Eric Firing (University of Hawaii) and Teri Chereskin (Scripps Institution of Oceanography). Data is collected on both the LMG and the NBP for the benefit of scientists on individual cruises, and for the long-term goal of building a profile of current structure in the Southern Ocean.

A data feed is sent from the ADCP system to RVDAS whenever a reference layer is acquired. This feed contains east and north vectors for ship's speed, relative to the reference layer, and ship's heading. Collected files (one per day) are archived in `0806adcp.tar` in the directory `/rvdas/nav`.

pCO₂

The NBP carries a pCO₂ measurement system from Lamont-Doherty Earth Observatory (LDEO). pCO₂ data is recorded by RVDAS and transmitted to LDEO at the end of each cruise. You will find pCO₂ data in a file named `0806pco2.tar` in the `/process` directory, which contains the pCO₂ instrument's data merged with GPS, meteorological and other oceanographic measurements. For more information contact Colm Sweeney (csweeney@ldeo.columbia.edu).

Cruise Science

CTD

The ctd data has been placed in the tar file `/ocean/0806ctd.tar`. The archive contains tar files `0806proc.tar`.

XBT

During the cruise, eXpendable BathyThermographs were used to obtain water column temperature profiles, providing corrections to the sound velocity profile for the multibeam system. The data files from these launches are included as `0806xbt.tar` in the `/ocean` directory.

Mocness

Multiple Opening Closing Net Environmental Sensing System (MOCNESS). The mocness is a system of nets that can be opened and closed remotely from the deck. It is used to catch small marine organisms. All of the sensors on the Mocness are the same Seabird and Wetlabs sensors used on the CTD.

Nutrients

A summary report of the nutrient analysis from NBP0806 is provided in an excel spreadsheet in `/Nutrient/0806Nuts.tar`. This spreadsheet summarized the data found in the .OMN data file from the Lachat Quickchem 8000 Nutrient Analyzer, which are also provided in the archive `/Nutrient/0806OMN.tar`.

RVDAS

The Research Vessel Data Acquisition System (RVDAS) was developed at Lamont-Doherty Earth Observatory of Columbia University and has been in use on its research ship for many years. It has been extensively adapted for use on the USAP research vessels.

Daily data processing of the RVDAS data is performed to calibrate and convert values into useable units and as a quality-control on operation of the DAS. Raw and processed data sets from RVDAS are included in the data distribution. The tables below provide detailed information on the sensors and data. Be sure to read the “Significant Acquisition Events” section for important information about data acquisition during this cruise.

Sensors and Instruments

RVDAS data is divided into two general categories, *underway and navigation*. They can be found on the distribution media as subdirectories under the top level rvdas directory: */rvdas/uw*, and */rvdas/nav*. Processed oceanographic data is in the top level directory, */process*. Each instrument or sensor produces a data file named with its channel ID. Each data file is g-zipped to save space on the distribution media. Not all data types are collected every day or on every cruise.

The naming convention for data files produced by the sensors and instruments is

NBP[CruiseID][ChannelID].dDDD

Example: NBP0806.met1.d126

- The CruiseID is the numeric name of the cruise, in this case, NBP0806.
- The ChannelID is a 4-character code representing the system being logged. An example is “met1,” the designation for meteorology.
- DDD is the day of year the data was collected

Underway Sensors

Meteorology and Radiometry

Measurement	Channel ID	Collect. Status	Rate	Instrument
Air Temperature	met1	continuous	1 sec	R. M. Young 41372LC
Relative Humidity	met1	continuous	1 sec	
Wind Speed/Direction	met1	continuous	1 sec	R.M. Young 05106
Barometer	met1	continuous	1 sec	R.M. Young 61201
PIR (LW radiation)	eng1	continuous	1 sec	Eppler PIR
PSP (SW radiation)	met1	continuous	1 sec	Eppler PSP
PAR	met1	continuous	1 sec	BSI QSR-240
GUV	pguv	continuous	2 sec	BSI PUV-2511
PUV	pguv	not collected		BSI PUG-2500

Geophysics

Measurement	Channel ID	Collect. Status	Rate	Instrument
Gravimeter	grv1	continuous	10 sec*	LaCoste & Romberg
Magnetometer	mag1	continuous	15 sec	EG&G G-866
Bathymetry	bat1	not collected	Varies	ODEC Bathy 2000
Bathymetry	knu1	continuous	Varies	Knudsen 320B/R

Bathymetry	sim1	not collected	Varies	Simrad EK500 Sonar
------------	------	---------------	--------	--------------------

*Data is output every second but it only changes every 10 seconds.

Oceanography

Measurement	Channel ID	Collect. Status	Rate	Instrument
Conductivity	tsg1	Continuous	6 sec	SeaBird SBE-21
Salinity	tsg1	Continuous	6 sec	Calc. from pri. temp
Sea Surface Temp	tsg1	Continuous	6 sec	SeaBird 3-01/S
Fluorometry	flr1	Continuous	1 sec	Turner 10-AU-005
Transmissometry	hdas	Continuous	6 sec	WET Lab C-Star
pCO ₂	pco2	Continuous	70 sec	(LDEO)
ADCP	adcp	Continuous	varies	RD Instruments

Navigational Instruments

Measurement	Channel ID	Collect. Status	Rate	Instrument
Trimble GPS	PCOD	Continuous	1 sec	Trimble 20636-00SM
Gyro	gyr1	Continuous	0.2 sec	Yokogawa Gyro
SeaPath	seap	Continuous	1 sec	SeaPath 200

Data

Data is received from the RVDAS system via RS-232 serial connections. A time tag is added at the beginning of each line of data in the form,

```
yy+dd:hh:mm:ss.sss [data stream from instrument]
```

where

yy = two-digit year

ddd = day of year

hh = 2 digit hour of the day

mm = 2 digit minute

ss.sss = seconds

All times are reported in UTC.

The delimiters that separate fields in the raw data files are often spaces and commas but can be other characters such as : = @. Occasionally no delimiter is present. Care should be taken when reprocessing the data that the field's separations are clearly understood.

In the sections below a sample data string is shown, followed by a table that lists the data contained in the string.

Underway Data

Each section below describes a type of data file (file name extension in parentheses) followed by a typical line of data in the file. In the table(s) for each section is a description of the fields within each line of data. Note: most data files listed below will be included with each cruise's data distribution, however some types of files may be omitted if the instrument was not operating during the cruise. The available data files can be found in the /rvdas/uw directory on the distribution disc.

Sound Velocity Probe (svp1)

00+348:01:59:52.128 1539.40

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

Meteorology (met1)

01+322:00:03:27.306 04.5 292 010 05.7 294 010 0959.6 000.2 093.1

-000.1537 0001.0886 0012.8248

Field	Data	Units
1	RVDAS time tag	
2	Port anemometer speed (relative)	m/s
3	Port anemometer direction (relative)	deg
4	Port anemometer standard deviation	deg
5	Starboard anemometer speed (relative)	m/s
6	Starboard anemometer direction (relative)	deg
7	Starboard anemometer standard deviation	deg
8	Barometer	mBar
9	Air temperature	°C
10	Relative humidity	%
11	PSP (short wave radiation)*	mV
12	PIR (long wave radiation)*	mV
13	PAR (photosynthetically available radiation)*	mV

*See page 21 for calculations.

Gravimeter (grv1)

There are now two sets of fields output by the gravity meter. The data record is output once per second, and identified by "\$DAT" in the id field. A summary of sensor environmental data is output every ten seconds, identified by "%ENV" in the id field.

Data record (\$DAT):

05+194:00:00:27.995 \$DAT,2005/ 7/13, 0: 7: 7.36,194, 9050.37, 9050.06, 5410.86, -0.00, -0.01, -0.02, 0.00, 0.00, 0.70, 0.19, -0.12, -0.25, 0.00, -69.45711315, -54.32181487, 0.000, 285.200,

Field	Data	Conversion	Units
1	RVDAS time tag		
2	Text string (id field)	\$DAT for data record	

Field	Data	Conversion	Units
3	Date	YYYY/MM/DD	
4	Time	HH:MM:SS.SS	
5	Day of Year	DDD	
6	Gravity count	mgal = count x 1.0046 + offset	count
7	Spring Tension		CU
8	Beam Position	Volts x 750,000	
9	VCC		
10	AL		
11	AX		
12	VE		
13	AX2		
14	XACC2		
15	LACC2		
16	CROSS ACCEL		GAL
17	LONG ACCEL		GAL
18	EOTVOS CORR		MGAL
19	LONGITUDE		Degrees
20	LATITUDE		Degrees
21	HEADING		Degrees
22	VELOCITY		Knots

Environmental record (\$ENV)

05+183:19:13:10.945 %ENV,2005/ 7/ 2,19:19:52.16,183,S-036/V1.5, 3.34,
 47.19, 20.34,1.111840E-1,-0.57700,-0.10591, 0.40180, 2.55260, 0.43000, 1,
 300

Field	Data	Conversion	Units
1	RVDAS time tag		
2	Text string (id field)	\$ENV for environmental record	
3	Date	YYYY/MM/DD	
4	Time	HH:MM:SS.SS	
5	Day of Year	DDD	
6	Meter ID		
7	Meter Pressure		inch-Hg
8	Meter temp		°C
9	Ambient temp		°C
10	K-Factor		
11	VCC Coeff		
12	AL Coeff		
13	AX Coeff		
14	VE Coeff		
15	AX2 Coeff		
16	Serial Filter Length		Seconds
17	QC Filter Length		Seconds

Magnetometer (mag1)

99+099:00:00:23.203 % 0 98 235928 0? 372453

Field	Data	Units
1	RVDAS time tag	
2	% 0 denotes G-866 magnetometer	
3	Year-day	
4	Time	
5	0? Denotes high noise condition	
6	Magnetic data (last digit is 10 th 's place)	nT

Knudsen (knud)

99+099:00:18:19.775 HF,305.2,LF,304.3

Field	Data	Units
1	RVDAS time tag	
2	HF = High frequency flag (12 kHz)	
3	High frequency depth	meters
4	LF = Low frequency flag (3.5 kHz)	
5	Low frequency depth	meters

Simrad EM120 (mbdp)

Field	Data	Units
1	LDTDS	
2	\$EMDPT	
3	Depth (corrected)	Meters

Thermosalinograph (tsg1)

00+019:23:59:46.976 15A16CFC163F8C2C100

Field	Data	Units
1	RVDAS time tag	
2	Seabird hex string (see page 22 for conversion to real units)	

Fluorometer (flr1)

00+019:23:59:58.061 0 0818 :: 1/19/00 17:23:17 = 0.983 (RAW) 1.2 (C)

Field	Data	Units
1	RVDAS time tag	
2	Marker 0 to 8	
3	4-digit index	
4	Date	mm/dd/yy
5	Time	hh:mm:ss
6	Signal	
7	Signal units of measurement	
8	Cell temperature (if temperature compensation package is installed)	
9	Temperature units (if temperature compensation package is installed)	

pCO₂ (pco2)

00+021:23:59:43.190 2000021.99920 2382.4 984.2 30.73 50.8 345.9 334.1 -1.70 -
68.046 -144.446 Equil

Field	Data	Units
1	RVDAS time tag	
2	pCO ₂ time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temperature	°C
5	Barometer	MBar
6	Concentration	ppm
7	Equilibrated temperature	°C
8	pCO ₂ pressure	microAtm
9	Flow rate	ml / min
10	Source ID #	1 or 2 digits
11	Valve position	1 or 2 digits
12	Flow source (Equil = pCO ₂ measurement)	text

Engineering (eng1)

07+280:06:45:29.359 12.2655 16.29123 134.663 98.51914 83.71822 -
3.354797 45.38742 -0.149594 15.25094 15.08044 NAN

Field	Data	Units
1	RVDAS time tag	
2	Power Supply Voltage	
3	Internal Case Temperature	
4	Pump #1 flow rate	L/min
5	Pump #2 flow rate	L/min
6	Seismic air pressure	Lbs/sq-in
7	PIR case resistance	Kohm
8	PIR case ratiometric output	mV
9	Freezer #1 temperature	C
10	Freezer #2 temperature	C
11	Freezer #3 temperature	C

*See page 25 for PIR calculations.

Hydro-DAS (hdas)

07+280:00:00:19.352 12.16678 15.94557 244.7432 4432.954 61.5 66.5 80.5
63

Field	Data	Units
1	RVDAS time tag	
2	Supply voltage	
3	Panel temperature	

Field	Data	Units
4	Fluorometer	mV
5	Transmissometer	mV
6	Flow meter 1 frequency	Hz
7	Flow meter 2 frequency	Hz
8	Flow meter 3 frequency	Hz
9	Flow meter 4 frequency	Hz

Micro-TSG (mtsg)

07+280:00:00:48.058 -1.5017, 2.70111, 33.9692, 1440.723

Field	Data	Units
1	RVDAS time tag	
2	Temperature	C
3	Conductivity	s/m
4	Sound velocity	m/s

GUV Data (pguv)

07+288:00:00:45.399 101507 000049 .000226 1.627E0 5.253E0 5.831E-1
4.382E-2 6.811E0 1.479E-2 6.719E0 45.707 17.954

Field	Data	Units
1	RVDAS time tag	
2	Date	mmddyy
3	Time (UTC)	hhmmss
4	Ed0Gnd	V
5	Ed0320	uW (cm ² nm)
6	Ed0340	uW (cm ² nm)
7	Ed0313	uW (cm ² nm)
8	Ed0305	uW (cm ² nm)
9	Ed0380	uW (cm ² nm)
10	Ed0PAR	uE (cm ² nm)
11	Ed0395	uW (cm ² nm)

Remote Temperature (rtmp)

07+272:00:00:15.960 -1.7870

Field	Data	Units
1	RVDAS time tag	
2	Temperature at seawater intake	C

Ultrasonic Anemometer (wind)

07+271:00:09:34.240 _A,139,007.55,M,+330.77,-001.52,65,_01

Field	Data	Units
1	RVDAS time tag	
2	Code (unit identification)	
3	Wind direction	Degrees
4	Wind speed	m/s
5	Wind speed units (M=M/S)	
6	Sound speed	m/s
7	Temperature (sonic)	C
8	Status (0 = OK, 60 = OK and heated, other code = error state)	
9	Checksum	

Navigational Data

Seapath GPS (seap)

The Seapath GPS outputs the following data strings, four in NMEA format and two in proprietary PSXN format:

- GPZDA
- GPGGA
- GPVTG
- GPHDT
- [PSXN, 20](#)
- PSXN, 22
- PSXN, 23

GPZDA

02+253:00:00:00.772 \$GPZDA,235947.70,09,09,2002,,*7F

Field	Data	Units
1	RVDAS time tag	
2	\$GPZDA	
3	time	hhmmss.ss
4	Day	dd
5	Month	mm
6	Year	yyyy
7	(empty field)	
8	Checksum	

GPGGA

02+253:00:00:00.938

GPGGA,235947.70,6629.239059,S,06827.668899,W,1,07,1.0,11.81,M,,M,,*6F

Field	Data	Units
1	RVDAS time tag	
2	\$GPGGA	
3	time	hhmmss.ss
4	Latitude	ddmm.mmmmmm
5	N or S for north or south latitude	
6	Longitude	ddmm.mmmmmm
7	E or W for east or west longitude	
8	GPS quality indicator, 0=invalid, 1=GPS SPS, 2=DGPS, 3=PPS, 4=RTK, 5=float RTK, 6=dead reckoning	
9	number of satellites in use (00-99)	
10	HDOP	x.x
9	height above ellipsoid in meters	m.mm
11	M	
12	(empty field)	
13	M	
14	age of DGPS corrections in seconds	s.s

Field	Data	Units
15	DGPS reference station ID (0000-1023)	
16	Checksum	

GPVTG

02+253:00:00:00.940 \$INVTG,19.96,T,,M,4.9,N,,K,A*39

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	course over ground, degrees true	d.dd
4	T	
5	,	
6	M	
7	speed over ground in knots	k.k
8	N	
9	,	
10	K	
11	Mode	
12	Checksum	

GPHDT

02+253:00:00:00.941 \$GPHDT,20.62,T*23

Field	Data	Units
1	RVDAS time tag	
2	\$GPHDT	
3	Heading, degrees true	d.dd
4	T	
5	Checksum	

PSXN,20

02+253:00:00:00.942 \$PSXN,20,0.43,0.43*39

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	20	
4	Horizontal position & velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
5	Height & vertical velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
6	Heading quality: 0=normal, 1=reduced performance, 2=invalid data	
7	Roll & pitch quality: 0=normal, 1=reduced performance, 2=invalid data	
8	Checksum	

PSXN,22

02+253:00:00:00.942 \$PSXN,22,0.43,0.43*39

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	22	
4	gyro calibration value since system start-up in degrees	d.dd

Field	Data	Units
5	short term gyro offset in degrees	d.dd
6	Checksum	

PSXN,23

02+253:00:00:02.933 \$PSXN,23,0.47,0.57,20.62,0.03*0C

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	23	
4	roll in degrees, positive with port side up	d.dd
5	pitch in degrees, positive with bow up	d.dd
6	Heading, degrees true	d.dd
7	heave in meters, positive down	m.mm
8	Checksum	

Trimble (P-Code) GPS (PCOD)

The Trimble GPS, which formerly output Precise Position (*P-Code*) strings, but now only outputs Standard Position (*Civilian*) strings, outputs three NMEA standard data strings:

- Position fix (GGA)
- Latitude / longitude (GLL),
- Track and ground speed (VTG)

GGA: GPS Position Fix – Geoid/Ellipsoid

01+319:00:04:11.193 \$GPGGA,000410.312,6227.8068,S,06043.6738,W,1,06,1.0,
031.9,M,-017.4,M,,*49

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGGA	
3	UTC time at position	hhmmss.sss
4	Latitude	ddmm.mmm
5	North (N) or South (S)	
6	Longitude	ddmm.mmm
7	East (E) or West (W)	
8	GPS quality: 0 = Fix not available or invalid 1 = GPS, SPS mode, fix valid 2 = DGPS (differential GPS), SPS mode, fix valid 3 = P-CODE PPS mode, fix valid	
9	Number of GPS satellites used	
10	HDOP (horizontal dilution of precision)	
11	Antenna height	meters
12	M for meters	
13	Geoidal height	meters
14	M for meters	
15	Age of differential GPS data (no data in the sample string)	

Field	Data	Units
16	Differential reference station ID (no data in the sample string)	
17	Checksum (no delimiter before this field)	

GLL: GPS Latitude/Longitude

01+319:00:04:11.272 \$GPGLL,6227.8068,S,06043.6738,W,000410.312,A*32

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGLL	
3	Latitude	degrees
4	North or South	
5	Longitude	degrees
6	East or West	
7	UTC of position	hhmmss.sss
8	Status of data (A = valid)	
9	Checksum	

VTG: GPS Track and Ground Speed

01+319:00:04:11.273 \$GPVTG,138.8,T,126.0,M,000.0,N,000.0,K*49

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	Heading	degrees
4	Degrees true (T)	
5	Heading	degrees
6	Degrees magnetic (M)	
7	Ship speed	knots
8	N = knots	
9	Speed	km/hr
10	K = km per hour	
11	Checksum	

Gyro Compass (gyr1)

00+019:23:59:59.952 \$HEHDT 25034,-020*73

Field	Data	Units
1	RVDAS time tag	
2	\$HEHDT	
3	Heading, Degrees True	degrees
5	Checksum	

ADCP Course (adcp)

00+019:23:59:59.099 \$PUHAW,UVH,-1.48,-0.51,250.6

Field	Data	Units
1	RVDAS time tag	
2	\$PUHAW	
3	UVH (E-W, N-S, Heading)	
4	Ship Speed relative to reference layer, east vector	knots
5	Ship Speed relative to reference layer, north vector	knots

Field	Data	Units
6	Ship heading	degrees

Sound Velocity Probe (svp1)

00+348:01:59:52.128 1539.40

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

Processed Data

The processed data sets can be found in the /process directory and subdirectories. Note: many of the subdirectories contain intermediate datasets to facilitate further processing and are not intended to be end-products. Only the final product files and datasets are described below.

pCO2-merged

00+346:23:58:20.672 2000346.9991 2398.4 1008.4 0.01 45.4 350.3 342.6 15.77

Equil -43.6826 173.1997 15.51 33.90 0.33 5.28 9.05 1007.57 40.0 14.87 182.44

Field	Data	Units
1	RVDAS time tag	
2	pCO ₂ time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temperature	°C
5	Barometer	MBar
6	Concentration	ppm
7	Equilibrated temperature	°C
8	pCO ₂ pressure	microAtm
9	Flow rate	ml / min
10	Source ID #	1 or 2 digits
11	Valve position	1 or 2 digits
12	Flow source (Equil = pCO ₂ measurement)	text
13	RVDAS latitude	degrees
14	RVDAS longitude	degrees
15	TSG external temperature	°C
16	TSG salinity	PSU
17	TSG fluorometry	V
18	RVDAS true wind speed	m/s
19	RVDAS true wind direction	degrees
20	Barometric Pressure	mBars
21	Uncontaminated seawater pump flow rate	l/min
22	Speed over ground	knots
23	Course made good	degrees

tsgfl

00+075:00:00:04.467 -01.488 -01.720 02.6783 33.63748 1.002442 0.002442

Field	Data	Units
1	RVDAS time tag	
2	Internal water temperature	°C
3	Sea Surface Temperature	°C

Field	Data	Units
4	Conductivity	μ Siemens
5	Salinity	PSU
6	Fluorometry	V
7	Transmissivity	V

Calculations

The file `instcoef.txt` located in the / directory contains the calibration factors for shipboard instruments. This was the file used by the RVDAS processing software.

TSG

Raw TSG data is stored as a 20 byte (character) long hex string. Example:

00+019:23:59:46.976 15A16CFC163F8C2C100

Bytes	Data
1-4	Sensor Temperature (in wet lab)
5-8	Conductivity
9-14	Remote Temperature (near seawater intake)
15-18	Transmissometer voltage

The coefficients for temperature and conductivity sensors can be found the `instcoef.txt` file and on the calibrations sheets in the appendix.

Calculating Temperature – ITS-90

T = decimal equivalent of bytes 1-4
 Temperature Frequency: $f = T/19 + 2100$
 $\text{Temperature} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15$ (°C)

Calculating Conductivity – ITS-90

C = decimal equivalent of bytes 5-8
 Conductivity Frequency $f = \sqrt{C*2100+6250000}$
 $\text{Conductivity} = (g + hf^2 + if^3 + jf^4)/[10(1 + \delta t + \epsilon p)]$ (siemens/meter)
 t = temperature (°C); p = pressure (decibars); $\delta = Ct_{cor}$; $\epsilon = CP_{cor}$

Calculating Transmittance

$V_{dark} = 0.058$ V
 $V_{ref} = 4.765$ V
 t = decimal equivalent of bytes 18 - 20
 Transmissometer Voltage (V_{signal}) = t/819
 $\% \text{ Transmittance} = (V_{signal} - V_{dark}) / (V_{ref} - V_{dark})$

PAR

raw data = mV
 calibration scale = 6.27 V/($\mu\text{Einstiens/cm}^2\text{sec}$)
 offset (V_{dark}) = 0.1 mV
 $(\text{raw mV} - V_{dark})/\text{scale} \times 104 \text{ cm}^2/\text{m}^2 \times 10^{-3} \text{ V/mV} = \mu\text{Einstiens/m}^2\text{sec}$
 or
 $(\text{data mV} - 0.1 \text{ mV}) \times 1.65 (\mu\text{Einstiens/m}^2\text{sec})/\text{mV} = \mu\text{Einstiens/m}^2\text{sec}$

PSP

```
raw data = mV
calibration scale = 7.92 x 10-6 V/(W/m2)
data mV / (scale x 103 mV/V) = W/m2
or
data mV x 120.7 (W/m2)/V = W/m2
```

PIR

Coefficient `pirCoeff` for this cruise can be found in the `instcoef.txt` file. Variable `PIRr` is the PIR case resistance and `PIRmv` is the radiometric output, as described in the “eng1” file description. Hard-coded “C” coefficients are shown below:

```
C1=0.0010295
C2=0.0002391
C3=0.0000001568
C4=5.6704e-8
```

Calculations (extracted from the C code):

```
raw data = mV
calibration scale = 4.16 x 10-6 V/(W/m2)
data mV / (scale x 103 mV/V) = W/m2
or
data mV x 120.7 (W/m2)/V = W/m2
Rr = log(fabs(PIRr * 1000))
T = 1 / ( C1 + (C2 * Rr) + (C3 * Rr * Rr * Rr) )
Rin = ( (PIRmv * 1000) / pirCoeff) + (C4 * T * T * T * T )
```

Acquisition Problems and Events

This section lists problems with acquisition noted during this cruise including instrument failures, data acquisition system failures and any other factor affecting this data set. The format is ddd:hh:mm (ddd is year-day, hh is hour, and mm is minute). Times are reported in GMT.

Start	End	Description
153:11:31		Started data loggers in Argentinean EEZ at 68° West
114:06:50		Exited Argentinean EEZ
159:2100	15921:30	Sea wall intake was interrupted. Ocean data gaps.
180:01:03		Enter British EEZ (Falklands)
181:00:33		Exit British EEZ
181:01:54		Entered Argentinean EEZ
182:01:38		Stopped data loggers at limit of Chilean EEZ at 68° West

Appendix: Sensors and Calibrations

NBP0806 Shipboard Sensors:

<i>Sensor</i>	<i>Serial Number</i>	<i>Last Calibration</i>	<i>Comments</i>
Meteorology & Radiometers			
Stbd Anemometer (Gill Ultrasonic)	071739	5/15/2007	Installed 7/19/2007
Port Anemometer	WM 46263	6/30/2007	Installed 7/19/2007
Stbd Anemometer	WM 73682	6/30/2007	Installed 7/19/2007
Bridge Anemometer	WM 45835	2/28/2007	Bridge (center)
Barometer	01705	12/01/2006	Installed 5/26/2008
Humidity/Wet Temp	06134	9/29/2006	Installed 5/26/2008
PIR	32845F3	7/30/2007	Installed 4/14/2008
PSP	32850F3	7/26/2007	Installed 4/14/2008
Mast PAR	6356	8/8/2007	Installed 8/28/2007
GUV (Mast)	25110203113	3/18/2008	Installed 4/18/08
Underway			
TSG	2131020-3198	5/20/06	Installed 02/07/07
TSG Remote Temp (Primary)	3846730-0352	6/6/2007	Installed 7/15/2007
TSG Remote Temp (Secondary)	031267	4/12/2006	Installed 1/29/07
Micro TSG	4549120-0226	01/12/2008	Installed 5/26/2008
Fluorometer (Primary)	5333-FRXX	Un-calibrated	Installed 4/14/04
Fluorometer (Secondary)	AFL-044	5/31/2006	Installed 6/23/2007
Transmissometer	CST-557DR	12/20/2006	Installed 3/14/08

NBP0806 CTD Sensors:

Sensor	Serial #	Last Calibration Date	Comments
CTD Fish	094857-0232	9/26/2006	
CTD Fish Pressure	43528	9/26/2006	
CTD Deck Unit	11P47914-0768	n/a	
Primary Temperature Sensor	03P2186	1/10/2008	
Secondary Temperature Sensor	03P2308	1/10/2008	
Primary Conductivity Sensor	041852	01/26/2008	
Secondary Conductivity Sensor	041850	6/26/2007	Noticed drift after cast 006 replaced with sensor 041314

Sensor	Serial #	Last Calibration Date	Comments
Secondary Conductivity Sensor	041314		Starting with cast 007
Dissolved Oxygen Sensor (Primary)	0082	1/9/2008	
Dissolved Oxygen Sensor (Secondary)	0080	7/25/07	
Fluorometer	AFL-016D	10/16/2006	Needed as spare for next cruise
Transmissometer	CST-889DR	7/27/2007	
CTD Pump (Primary)	051626	4/17/2008	In House Cal
CTD Pump (Secondary)	051646	4/17/2008	In House Cal
Altimeter	497	n/a	
Slip Ring Assembly	n/a	n/a	
Carousel Water Sampler	3211265-0066	n/a	

NBP0806 MOCNESS Sensors:

Sensor	Serial #	Last Calibration Date	Comments
Temperature Sensor	034080	6/11/2005	Seabird SBE -35
Primary Conductivity Sensor	041431	1/26/2008	Seabird SBEE 4-o2/0
Fluorometer	AFL-011	2/14/2008	WetLabs AFLT
Transmissometer	CST-439DR	11/14/2007	WetLabs C-Star

Note:

There originally was another temperature sensor on the Mocness. It was bad from the onset and never recorded any data. It is not listed here.

Calibrations

The following pages are replicas of current calibration sheets for the sensors used during this cruise.

Gravity Tie Spreadsheet

United States Antarctic Program

Meteorology System

Anemometer (Port)

RM Young Anemometer Calibration, Model 05106

S/N: 46263

Date: 30-Jun-07

Cal'd By: George Aukon

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.10	-0.10	0.0
200	0.98	0.90	0.08	1.9
500	2.45	2.30	0.15	4.8
1000	4.90	4.80	0.10	9.5
1500	7.35	7.30	0.05	14.3
2000	9.80	9.80	0.00	19.0
3000	14.70	14.70	0.00	28.6
4000	19.60	19.60	0.00	38.1
5000	24.50	24.60	-0.10	47.6
6000	29.40	29.40	0.00	57.1
7000	34.30	34.30	0.00	66.6
8000	39.20	39.40	-0.20	76.2
9000	44.10	44.20	-0.10	85.7
10000	49.00	49.10	-0.10	95.2
12000	58.80	58.90	-0.10	114.2

Direction	Measured Direction	Delta Direction
0	0	0
30	30	0
60	59	1
90	89	1
120	118	2
150	148	2
180	179	1
210	210	0
240	240	0
270	270	0
300	300	0
330	330	0
0	0	0

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.10	-0.10
200	0.98	0.80	0.18
500	2.45	2.40	0.05
1000	4.90	4.80	0.10
1500	7.35	7.30	0.05
2000	9.80	9.80	0.00
3000	14.70	14.70	0.00
4000	19.60	19.60	0.00
5000	24.50	24.60	-0.10
6000	29.40	29.50	-0.10
7000	34.30	34.40	-0.10
8000	39.20	39.30	-0.10
9000	44.10	44.30	-0.20
10000	49.00	49.20	-0.20
12000	58.80	58.90	-0.10

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm?	2
Wind Direction Threshold < 30 gm?	15

Additional Comments

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

Anemometer (Starboard)**RM Young Anemometer Calibration, Model 05106**

S/N: 73682

Date: 30-Jun-07

Cal'd By: George Aukon

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.10	-0.10	0.0
200	0.98	0.80	0.18	1.9
500	2.45	2.40	0.05	4.8
1000	4.90	4.80	0.10	9.5
1500	7.35	7.30	0.05	14.3
2000	9.80	9.80	0.00	19.0
3000	14.70	14.70	0.00	28.6
4000	19.60	19.60	0.00	38.1
5000	24.50	24.60	-0.10	47.6
6000	29.40	29.50	-0.10	57.1
7000	34.30	34.40	-0.10	66.6
8000	39.20	39.30	-0.10	76.2
9000	44.10	44.30	-0.20	85.7
10000	49.00	49.20	-0.20	95.2
12000	58.80	58.90	-0.10	114.2

Direction	Measured Direction	Delta Direction
0	0	0
30	29	1
60	59	1
90	89	1
120	119	1
150	148	2
180	178	2
210	207	3
240	237	3
270	267	3
300	297	3
330	328	2
0	0	0

Note: Delta direction should not exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.10	-0.10
200	0.98	0.90	0.08
500	2.45	2.30	0.15
1000	4.90	4.80	0.10
1500	7.35	7.30	0.05
2000	9.80	9.80	0.00
3000	14.70	14.70	0.00
4000	19.60	19.60	0.00
5000	24.50	24.60	-0.10
6000	29.40	29.40	0.00
7000	34.30	34.30	0.00
8000	39.20	39.40	-0.20
9000	44.10	44.20	-0.10
10000	49.00	49.10	-0.10
12000	58.80	58.90	-0.10

Caution: Do Not exceed 12000 rpm during Wind Speed test.

Wind Speed Threshold < 2.9 gm? 2.3
Wind Direction Threshold < 30 gm? 15

Additional Comments

Note: Delta Windspeed should not exceed + or - 0.3 m/s for 0 - 5000 rpm

Anemometer (Bridge)**RM Young Anemometer Calibration, Model 05106**

S/N: 45835

Date: 28-Feb-07

Cal'd By: George Aukon

Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s	Knots
0	0.00	0.00	0.00	0.0
200	0.98	0.90	0.08	1.9
500	2.45	2.40	0.05	4.8
1000	4.90	4.80	0.10	9.5
1500	7.35	7.30	0.05	14.3
2000	9.80	9.80	0.00	19.0
3000	14.70	14.60	0.10	28.6
4000	19.60	19.50	0.10	38.1
5000	24.50	24.30	0.20	47.6
6000	29.40	29.20	0.20	57.1
7000	34.30	34.10	0.20	66.6
8000	39.20	39.00	0.20	76.2
9000	44.10	43.90	0.20	85.7
10000	49.00	48.80	0.20	95.2
12000	58.80	58.60	0.20	114.2

Direction	Measured Direction	Delta Direction
0	359	0
30	29	1
60	59	1
90	89	1
120	119	1
150	148	2
180	179	1
210	210	0
240	240	0
270	270	0
300	301	-1
330	331	-1
0	1	-1

Note: Delta direction should not
exceed + or - 3 degrees.

Counter Clockwise Cal Motor RPM	Calculated Windspeed m/s	Measured Windspeed m/s	Delta m/s
0	0.00	0.00	0.00
200	0.98	1.00	-0.02
500	2.45	2.50	-0.05
1000	4.90	4.90	0.00
1500	7.35	7.40	-0.05
2000	9.80	9.80	0.00
3000	14.70	14.80	-0.10
4000	19.60	19.80	-0.20
5000	24.50	24.60	-0.10
6000	29.40	29.50	-0.10
7000	34.30	34.50	-0.20
8000	39.20	39.40	-0.20
9000	44.10	44.40	-0.30
10000	49.00	49.30	-0.30
12000	58.80	59.60	-0.80

Caution: Do Not exceed 12000 rpm during Wind
Speed test.

Wind Speed Threshold < 2.9 gm? ☒ yes
Wind Direction Threshold < 30 gm? ☒ yes

Additional Comments

Potentiometer and potentiometer coupling
were replaced, vertical shaft bearings were
cleaned and lubricated.

Note: Delta Windspeed should not exceed
+ or - 0.3 m/s for 0 - 5000 rpm

Barometer

R.M. Young Company
2801 Aero Park Drive
Traverse City, Michigan 49686 USA

Barometric Pressure Sensor Calibration Report

Customer: *Raytheon Technical Services Co*

Test Number: 60621

Customer PO: RM31245-50

Test Date: 1 December 2006

Sales Order: 8800

Test Sensor:

Model: 61201

Serial Number: BP01705

Description: Barometric Pressure Sensor

Report of calibration comparison of test barometric pressure sensor with National Institute of Standards and Technology traceable standard pressure calibrator at five pressures in the R.M. Young Company controlled pressure facility. Calibration accuracy ± 1.0 hPa.

Reference Pressure (hPa)	Voltage Output (millivolts)	Indicated (1) Pressure (hPa)
800.0	0	800.0
875.0	1251	875.1
950.0	2501	950.1
1025.0	3750	1025.0
1100.0	4998	1099.9

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument

Druck Pressure Controller Model DPI515
Fluke Multimeter Model 8060A

Serial # NIST Test Reference

51500497 UKAS Lab 0221
4865407 234027

Tested By: *E. Chumney*

METEOROLOGICAL INSTRUMENTS

Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com

Humidity Sensor

R.M. Young Company
2801 Aero Park Drive
Traverse City, Michigan 49686 USA

3-04
COPY

Relative Humidity Sensor Calibration Report

Customer: *Raytheon Technical Services Co LLC*

Test Number: 69292R
Test Date: 29 September 2006

Customer PO: RM29548.50
Sales Order: 8708

Test Sensor:

Model: 41372LC Serial Number: 6134
Description: Temperature/Relative Humidity Sensor

Report of calibration comparison of test relative humidity sensor with National Institute of Standards and Technology traceable standard relative humidity sensor at five humidity levels in the R.M. Young Company controlled humidity chamber facility. Calibration accuracy ± 2.0 %.

Reference Humidity (%)	Current Output (milliamps)	Indicated (1) Humidity (%)
10.4	5.9	11.9
30.4	8.8	30.2
49.7	12.0	50.0
69.9	15.2	69.8
89.6	17.9	86.6

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument

Vaisala Humidity Sensor Model 35AC
Fluke Multimeter Model 8060A

Serial # NIST Test Reference

N475040 TN 266152
4865407 234027

Tested By: *E. Channing*

page 2

METEOROLOGICAL INSTRUMENTS

Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com

Temperature Sensor

R.M. Young Company
2801 Aero Park Drive
Traverse City, Michigan 49686 USA

3-04
met

**Temperature Sensor Calibration Report**

Customer: **Raytheon Technical Services Co LLC**

Test Number: 69292 Customer PO: RM29548-50
Test Date: 29 September 2006 Sales Order: 8708

Test Sensor:

Model: 41372LC Serial Number: 6134
Description: Temperature/Relative Humidity Sensor

Report of calibration comparison of test temperature sensor with National Institute of Standards and Technology traceable standard thermometers at three temperatures in the R.M. Young Company controlled temperature calibration bath facilities. Calibration accuracy $\pm 0.1^\circ$ Celsius.

Bath Temperature (degrees C)	Current Output (milliamps)	Indicated (1) Temperature (degrees C)
-50.03	3.992	-50.05
0.03	12.003	0.02
50.03	20.004	50.03

(1) Calculated from current output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument	Serial #	NIST Test Reference
Brooklyn Thermometer Model 43-FC	8006-118	204365
Brooklyn Thermometer Model 22332-D5-FC	25071	249763
Brooklyn Thermometer Model 2X400-D7-FC	77532	228060
Keithley Multimeter Model 191	15232	234027

Tested By:

EChenning

page 1

METEOROLOGICAL INSTRUMENTS

Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com

PIR**THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA
Telephone: 401-847-1020 Fax: 401-847-1031
Email: info@eppleylab.com Internet: www.eppleylab.com



Scientific Instruments
for Precision Measurements
Since 1917

**STANDARDIZATION OF
EPPLEY PRECISION INFRARED RADIOMETER
Model PIR**

Serial Number: 32845F3

Resistance: 740 Ω at 23 $^{\circ}\text{C}$
Temperature Compensation Range: -20 to 40 $^{\circ}\text{C}$

This pyrgeometer has been compared against Eppley's Blackbody Calibration System under radiation intensities of approximately 200 watts meter⁻² and an average ambient temperature of $^{\circ}\text{C}$ as measured by Standard Omega Temperature Probe, RTD#1.

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$4.16 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 700 watts meter⁻². This radiometer is linear to within $\pm 1.0\%$ up to this intensity.

The calibration of this instrument is traceable to the International Practical Temperature Scale (ITS) through a precision low-temperature blackbody.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".

Shipped to:
National Science Foundation
Port Hueneme, CA

S.O. Number: 61242
Date: August 1, 2007

Date of Test: July 30, 2007

In Charge of Test:

Reviewed by:

Remarks:

PSP**THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA

Telephone: 401-847-1020

Fax: 401-847-1031

Email: info@eppleylab.com

Internet: www.eppleylab.com

EPLABScientific Instruments
for Precision Measurements
Since 1917**STANDARDIZATION OF
EPPLEY PRECISION SPECTRAL PYRANOMETER
Model PSP**

Serial Number: 32850F3

Resistance: 706 Ω at 23 $^{\circ}\text{C}$
Temperature Compensation Range: -20 to 40 $^{\circ}\text{C}$

This radiometer has been compared with Standard Precision Spectral Pyranometer, Serial Number 21231F3 in Eppley's Integrating Hemisphere under radiation intensities of approximately 700 watts meter⁻² (roughly one half a solar constant).

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$7.92 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 1400 watts meter⁻². This radiometer is linear to within $\pm 0.5\%$ up to this intensity.

The calibration of this instrument is traceable to standard self-calibrating cavity pyrheliometers in terms of the Systems Internationale des Unites (SI units), which participated in the Tenth International Pyrheliometric Comparisons (IPC X) at Davos, Switzerland in September-October 2005.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".

Useful conversion facts: 1 cal cm⁻² min⁻¹ = 697.3 watts meter⁻²
1 BTU/ft²-hr⁻¹ = 3.153 watts meter⁻²

Shipped to:
National Science Foundation
Port Hueneme, CA

S.O. Number: 61243
Date: August 1, 2007

Date of Test: July 26, 2007

In Charge of Test:

Reviewed by:

Remarks:

PAR**Biospherical Instruments Inc.****CALIBRATION CERTIFICATE**

Calibration Date 8/8/2007
Model Number QSR-240
Serial Number 6356
Operator TPC
Standard Lamp HEC-1630(10/25/2006)
Probe Excitation Voltage Range: 6 to 18 VDC(+)
Output Polarity: Positive

Probe Conditions at Calibration(In air):

Calibration Voltage: 6 VDC(+)
Probe Current: 1.2 mA

Probe Output Voltage:

Probe Illuminated 93.1 mV
Probe Dark -0.1 mV
Probe Net Response 93.1 mV
RG780 Filter 0.1 mV

Corrected Lamp Output:

Output In Air (same condition as calibration):

9.56E+15 quanta/cm²sec
0.01588 uE/cm²sec

Calibration Scale Factor:

(To calculate irradiance, divide the net voltage reading in Volts by this value.)

Dry: 9.7383E-18 V/(quanta/cm²sec)
5.8644E+00 V/(uE/cm²sec)

Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with alcohol.
4. Calibration was performed with customer cable, when available.

QSR240R 05/24/95

GUV

Biospherical Instruments Inc.

GUV-2511 Calibration Certificate

System Serial Number		25110203113				Date of Calibration		3/18/08			
Calibration database		25110203113v4.mdb				Date of Certificate		3/18/2008			
DASSN		0068				Standard of Spectral Irradiance		91537(10/25/06)			
Microprocessor Tag Number		2				Operator		TC			
Monochromatic Channels		Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	ScaleSmall [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	ScaleMedium [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	ScaleLarge [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
Ed0320		2	320	2.7010E-10	2.7551E-05	8.0491E-03	2.8497E+00	6.5000E-05	6.4000E-05	2.2300E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0340		6	340	2.2027E-10	2.2467E-05	6.5640E-03	2.3144E+00	3.7400E-04	3.7600E-04	1.1590E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0313		8	313	2.4100E-10	2.4539E-05	7.1692E-03	2.5594E+00	1.0000E-04	1.0000E-04	6.9100E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0305		10	305	1.6600E-11	1.6943E-06	4.9499E-04	1.5313E-01	4.1300E-04	4.0500E-04	-2.2080E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0380		12	380	7.0759E-11	7.2174E-06	2.1086E-03	7.0320E-01	1.1140E-03	1.1050E-03	-1.4780E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0395		18	395	3.4926E-10	3.5624E-05	1.0408E-02	3.3997E+00	1.3100E-04	1.3000E-04	2.2300E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Broadband Channels		Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	ScaleSmall [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	ScaleMedium [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	ScaleLarge [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
Ed0PAR		13	400-700	1.9205E-05	1.9589E+00	5.7230E+02	2.0376E+05	8.8600E-04	8.7700E-04	-1.3030E-03	$\mu\text{E}/(\text{cm}^2\cdot\text{sec})$
Auxiliary Channels		Address	Wavelength	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement Units
Ed0Gnd		0	0	1	1	1	1	0	0	0	V
Ed0Temp		22	0	1	0.01	0.01	0.01	0	0	0	C
Ed0Vin		27	0	1	-0.25	-0.25	-0.25	0	0	0	V

© Biospherical Instruments Inc., 5340 Riley Street, San Diego, California 92110 USA. Contact support@biospherical.com for more information.

TSG Calibration Files

Underway Conductivity

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 3198
 CALIBRATION DATE: 20-May-06

SBE21 CONDUCTIVITY CALIBRATION DATA
 PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHIJ COEFFICIENTS

g = -4.27061383e+000
 h = 5.04384737e-001
 i = -4.53257393e-004
 j = 4.72934991e-005
 CPcor = -9.5700e-008 (nominal)
 CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 2.81077465e-006
 b = 5.02715558e-001
 c = -4.26259709e+000
 d = -8.83813520e-005
 m = 4.8
 CPcor = -9.5700e-008 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2.91246	0.00000	0.00000
1.0000	34.8123	2.97566	8.21793	2.97567	0.00002
4.6261	34.7919	3.29397	8.59263	3.29396	-0.00001
15.0000	34.7503	4.26437	9.64425	4.26434	-0.00003
18.4999	34.7417	4.60953	9.99119	4.60955	0.00002
24.0000	34.7323	5.16751	10.52728	5.16752	0.00001
29.0000	34.7279	5.68947	11.00456	5.68948	0.00001
32.4999	34.7263	6.06206	11.33261	6.06205	-0.00001

Conductivity = $(g + hf^2 + if^3 + jf^4) / [10(1 + \delta t + \epsilon p)]$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

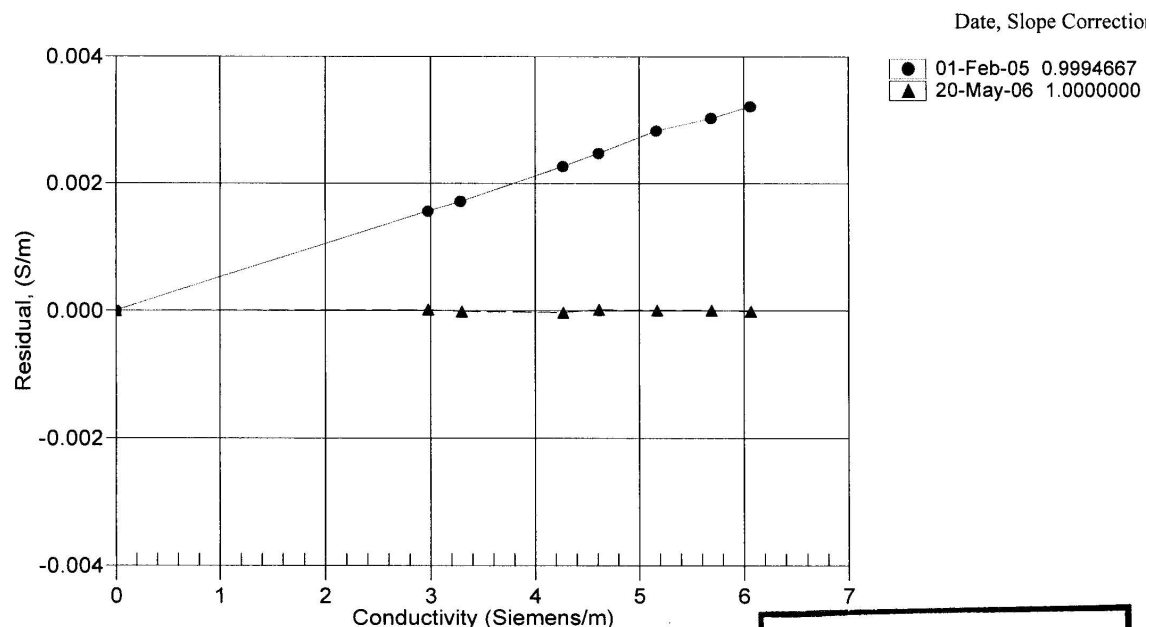

**POST CRUISE
CALIBRATION**

Underway Temperature Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 3198
CALIBRATION DATE: 20-May-06SBE21 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

ITS-90 COEFFICIENTS

$g = 4.22473160e-003$
 $h = 6.29770835e-004$
 $i = 2.05272425e-005$
 $j = 1.54706370e-006$
 $f0 = 1000.0$

ITS-68 COEFFICIENTS


$a = 3.64763347e-003$
 $b = 5.95315785e-004$
 $c = 1.61762223e-005$
 $d = 1.54852177e-006$
 $f0 = 2568.439$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	2568.439	1.0001	0.00011
4.6261	2782.830	4.6259	-0.00021
15.0000	3467.526	15.0002	0.00020
18.4999	3723.433	18.5000	0.00006
24.0000	4152.193	23.9998	-0.00023
29.0000	4571.111	29.0000	0.00004
32.4999	4881.298	32.4999	0.00004

$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS: T_{68} is assumed to be $1.00024 * T_{90}$ (-2 to 35 $^\circ\text{C}$)

Residual = instrument temperature - bath temperature

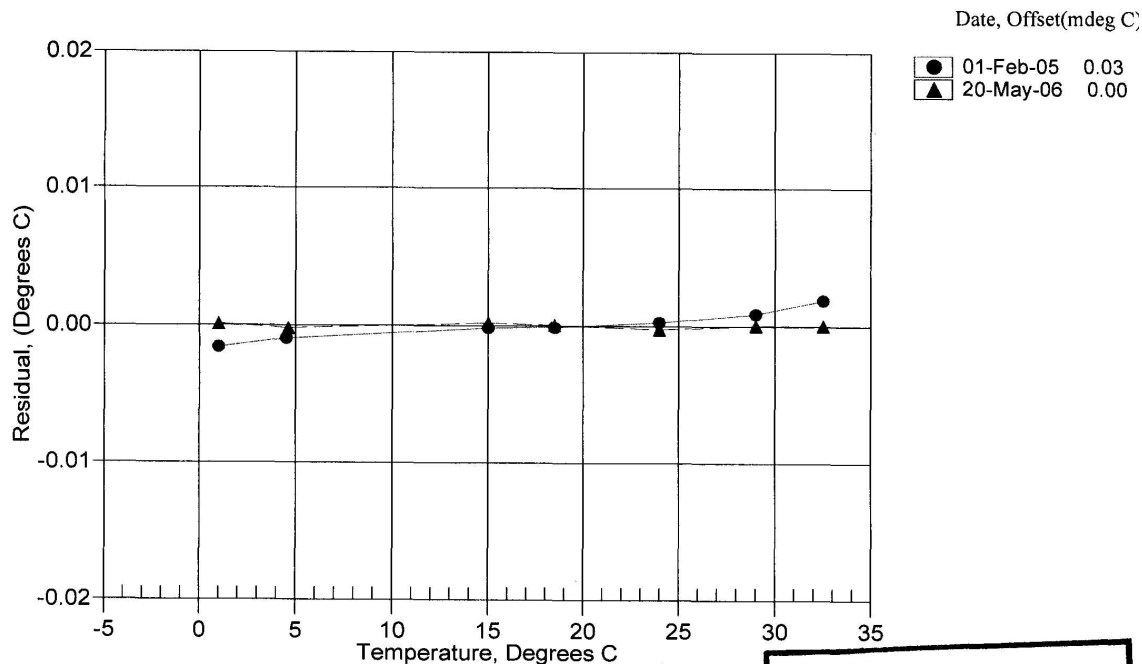
**POST CRUISE
CALIBRATION**

Underway Temperature Sensor (Primary Remote)

44

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0352
CALIBRATION DATE: 06-Jun-07SBE 38 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE


ITS-90 COEFFICIENTS

 $a_0 = -1.791146e-005$
 $a_1 = 2.748666e-004$
 $a_2 = -2.288718e-006$
 $a_3 = 1.522128e-007$

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.50010	809858.1	-1.50005	0.00005
0.99990	723216.3	0.99986	+0.00004
4.50000	619038.5	4.49993	+0.00007
7.99990	531605.5	7.99989	+0.00001
11.50000	457969.9	11.50002	0.00002
14.99990	395755.0	15.00000	0.00010
18.49990	343018.4	18.49995	0.00005
22.00000	298175.3	21.99994	+0.00006
25.50000	259928.8	25.49995	+0.00005
29.00000	227212.0	28.99995	-0.00005
32.50000	199144.2	32.50006	0.00006

$$\text{Temperature ITS-90} = 1/(a_0 + a_1 \ln(n)) + a_2 [\ln(n)]^2 + a_3 [\ln(n)]^3 - 273.15 \text{ (}^\circ\text{C)}$$

Residual = instrument temperature - bath temperature

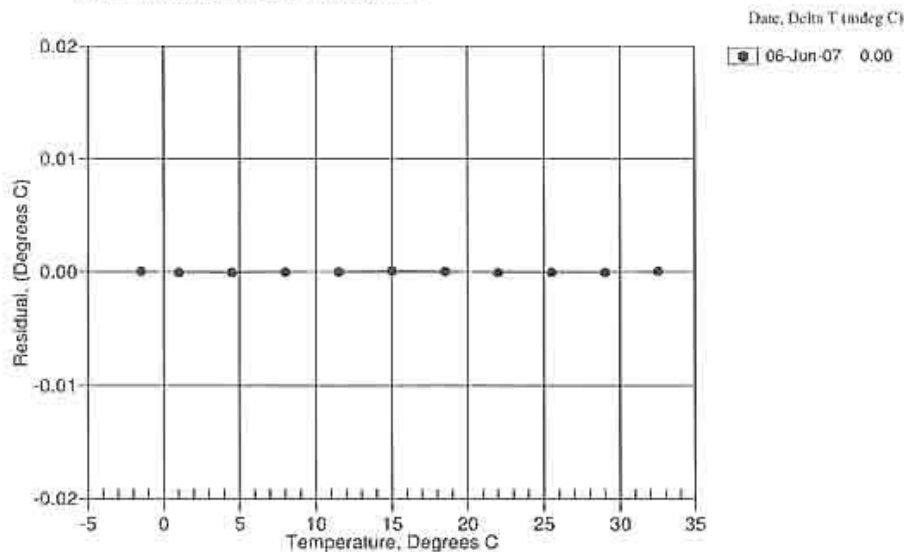

Underway Temperature Sensor (Secondary Remote)**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1267
CALIBRATION DATE: 12-Apr-06SBE3 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

ITS-90 COEFFICIENTS

$g = 4.76625066e-003$
 $h = 6.64522185e-004$
 $i = 2.84261863e-005$
 $j = 2.62601374e-006$
 $f_0 = 1000.0$

ITS-68 COEFFICIENTS


$a = 3.68121498e-003$
 $b = 5.89543636e-004$
 $c = 1.47312260e-005$
 $d = 2.62748536e-006$
 $f_0 = 5707.029$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5001	5707.029	-1.5002	-0.00010
1.0000	6042.027	1.0001	0.00005
4.4999	6534.652	4.5000	0.00014
7.9999	7055.608	8.0000	0.00007
11.4999	7605.659	11.4998	-0.00008
14.9999	8185.578	14.9998	-0.00014
18.4999	8796.088	18.4998	-0.00011
22.0000	9437.895	22.0000	-0.00003
25.4999	10111.624	25.5001	0.00019
28.9999	10817.898	29.0001	0.00019
32.4999	11557.257	32.4997	-0.00019

$$\text{Temperature ITS-90} = 1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature ITS-68} = 1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS: T_{68} is assumed to be $1.00024 * T_{90}$ (-2 to 35 $^\circ\text{C}$)

Residual = instrument temperature - bath temperature

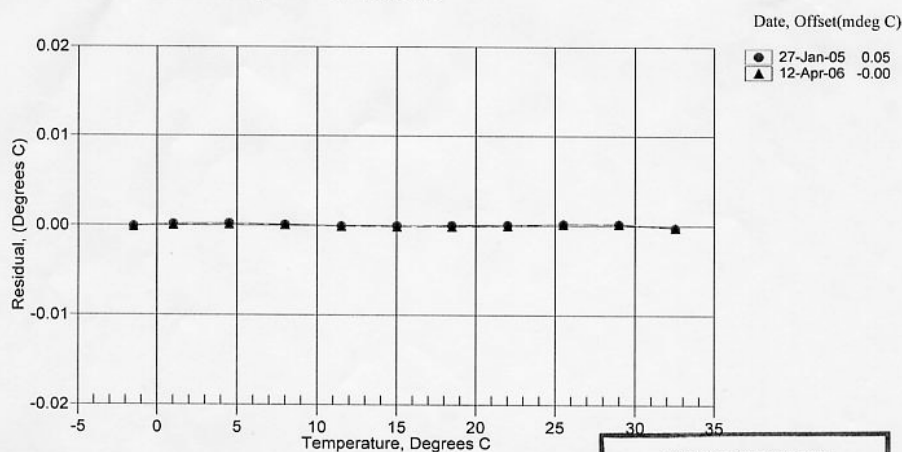**POST CRUISE
CALIBRATION**

Micro-TSG Calibration Files***Temperature Sensor (Micro-TSG)***

Sensor Serial No: 0226

Sea Bird Electronics, Inc
1808 136th Place NE
Bellevue, WA 98005

Conductivity Sensor (Micro-TSG)

Sensor Serial No: 0226

Sea Bird Electronics, Inc
1808 136th Place NE
Bellevue, WA 98005

Underway fluorometer (Primary)

PO Box 518
620 Applegate St.
Philomath OR 97370



(541) 929-5650
Fax (541) 929-5277
<http://www.wetlabs.com>

Chlorophyll Fluorometer Characterization

Date: 05/31/06
Serial #: AFL-044
Job#: 0209007
Tech: K.C

Dark Counts 0.177 volts
CEV 2.725 volts
SF 9.8116

FSV 5.45 volts

Linearity: 0.999 R² (0–1.5 volts)
0.995 R² (0– 5.45 volts)

Notes:

Dark Counts: Signal output of the meter in clean water with black tape over detector.

CEV is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to **25 µg/l** of a *Thalassiosira weissflogii* phytoplankton culture.

SF is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determined by using the following equation:
 $SF = (25) / (CEV - \text{dark})$ e.g. $(25) / (2.865 - 0.238) = 9.516$

FSV is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m³) can be derived by using the following equation: (µg/l) = (V_{measured} – CWO) * SF

The relationship between fluorescence and chlorophyll-*a* concentrations in-situ is highly variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

Underway Transmissometer

PO Box 518
620 Applegate St.
Philomath, OR 97370



(541) 929-5650
Fax (541) 929-5277
www.wetlabs.com

C-Star Calibration and Repairs

Date	12/20/2006	Customer	Raytheon Polar Services
Job #	021020	S/N#	CST-557DR
		Work order	007

Repairs and Modifications:

Replaced bulkhead connector, 38 mm lens and o-rings. Baked to remove moisture. Recalibrated.

Comments:

- Shake-tested unit
- Pressure-tested unit
- Noise test: 1 sample/sec for 60 sec
- Stability test: 1 sample/min for 12 hrs
- Performed water calibration
- Temperature test, 27–2 °C
- Updated unit's calibration sheet

cstarwkbkf1.xls

Revision F

6/12/03

CTD Pressure Sensor (fish)**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0232
CALIBRATION DATE: 26-Sep-06SBE9plus PRESSURE CALIBRATION DATA
10000 psia S/N 43528

DIGIQUARTZ COEFFICIENTS:


C1 = -5.103000e+004
 C2 = 8.606365e-002
 C3 = 1.481220e-002
 D1 = 3.642300e-002
 D2 = 0.000000e+000
 T1 = 3.004925e+001
 T2 = -3.406308e-004
 T3 = 4.125600e-006
 T4 = 1.811600e-009
 T5 = 0.000000e+000

AD590M, AD590B, SLOPE AND OFFSET:

AD590M = 1.13600e-002
 AD590B = -8.42350e+000
 Slope = 0.99978
 Offset = 0.0319 (dbars)

PRESSURE (PSIA)	INST OUTPUT(Hz)	INST TEMP(C)	INST OUTPUT (PSIA)	CORRECTED INST OUTPUT (PSIA)	RESIDUAL (PSIA)
14.675	33289.50	21.9	14.568	14.615	-0.060
2001.705	33930.70	22.1	2002.284	2001.886	0.181
3988.395	34558.00	22.1	3989.251	3988.409	0.014
5975.164	35172.50	22.2	5976.527	5975.241	0.077
7962.097	35774.80	22.2	7963.884	7962.154	0.057
9949.272	36365.50	22.3	9951.215	9949.041	-0.231
7961.761	35774.70	22.4	7963.436	7961.706	-0.055
5974.924	35172.50	22.5	5976.351	5975.065	0.141
3988.024	34558.00	22.5	3988.996	3988.154	0.130
2001.221	33930.60	22.6	2001.645	2001.247	0.026
14.671	33289.60	22.9	14.346	14.392	-0.279

Residual = corrected instrument pressure - reference pressure

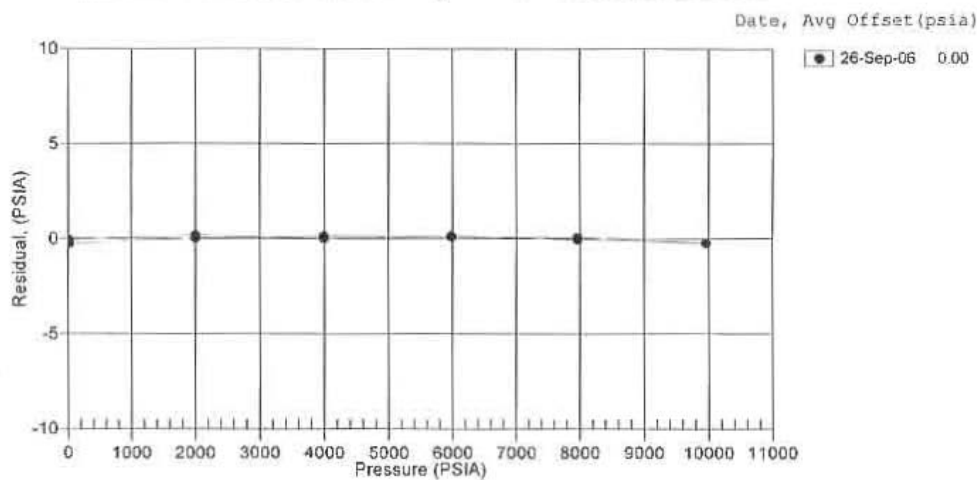

CTD Primary Temperature Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2186
CALIBRATION DATE: 10-Jan-08SBE3 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

ITS-90 COEFFICIENTS

$g = 4.34004885e-003$
 $h = 6.44357902e-004$
 $i = 2.30359279e-005$
 $j = 2.14466833e-006$
 $f0 = 1000.0$

IPTS-68 COEFFICIENTS


$a = 3.68121353e-003$
 $b = 6.02943002e-004$
 $c = 1.62526134e-005$
 $d = 2.14621884e-006$
 $f0 = 2882.302$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5001	2882.302	-1.5001	0.00001
0.9999	3047.621	0.9999	-0.00001
4.4999	3290.441	4.4999	-0.00003
7.9999	3546.873	7.9999	0.00000
11.4999	3817.278	11.4999	0.00004
14.9999	4102.010	15.0000	0.00005
18.4999	4401.404	18.4999	-0.00005
21.9999	4715.808	21.9998	-0.00009
25.4999	5045.555	25.4999	0.00004
28.9999	5390.931	29.0000	0.00009
32.4999	5752.220	32.4999	-0.00005

$$\text{Temperature ITS-90} = 1/[g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]] - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature IPTS-68} = 1/[a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]] - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS: T_{68} is assumed to be $1.00024 * T_{90}$ (-2 to 35 $^\circ\text{C}$)

Residual = instrument temperature - bath temperature

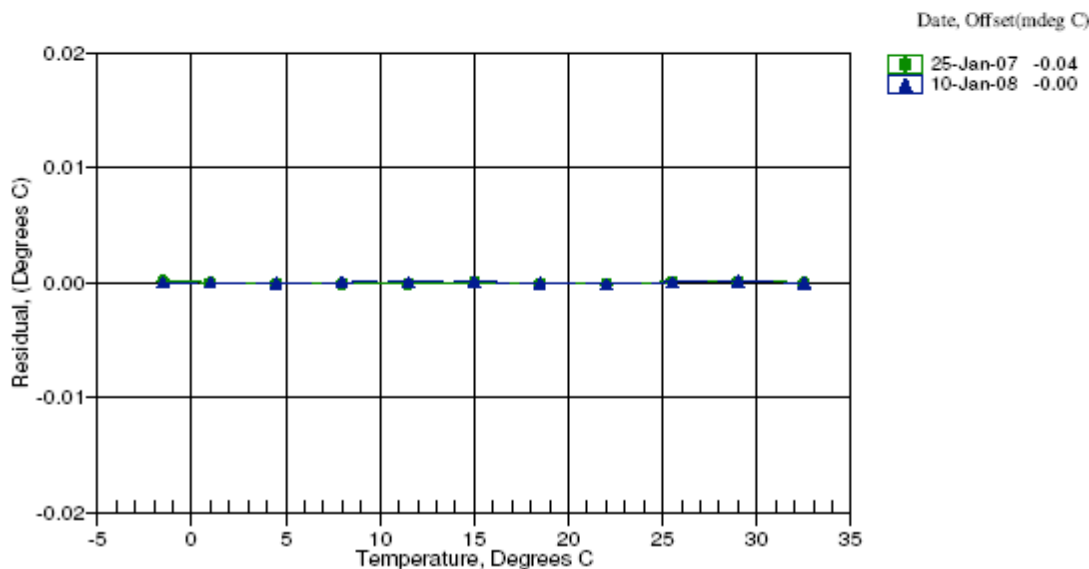

**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Temperature Calibration Report

Customer:	Raytheon Polar Services Co.		
Job Number:	48653	Date of Report:	1/10/2008
Model Number:	SBE 03Plus	Serial Number:	03P2186

Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.

'AS RECEIVED CALIBRATION'☒ **Performed** ☐ **Not Performed**

Date: 1/10/2008

Drift since last cal: +0.00004 Degrees Celsius/year

Comments:

'CALIBRATION AFTER REPAIR'☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: Degrees Celsius/year

Comments:

CTD Secondary Temperature Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2308
CALIBRATION DATE: 10-Jan-08SBE3 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

ITS-90 COEFFICIENTS

$g = 4.34505775e-003$
 $h = 6.44550497e-004$
 $i = 2.32217908e-005$
 $j = 2.16913976e-006$
 $f0 = 1000.0$

IPTS-68 COEFFICIENTS


$a = 3.68121362e-003$
 $b = 6.02554500e-004$
 $c = 1.63069131e-005$
 $d = 2.17069685e-006$
 $f0 = 2906.243$

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5001	2906.243	-1.5001	0.00000
0.9999	3073.048	0.9999	0.00000
4.4999	3318.063	4.4999	-0.00003
7.9999	3576.831	7.9999	0.00000
11.4999	3849.717	11.4999	0.00003
14.9999	4137.079	14.9999	0.00003
18.4999	4439.261	18.4999	-0.00004
21.9999	4756.612	21.9998	-0.00006
25.4999	5089.463	25.4999	0.00003
28.9999	5438.111	29.0000	0.00006
32.4999	5802.850	32.4999	-0.00003

$$\text{Temperature ITS-90} = 1/[g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]] - 273.15 \text{ (}^\circ\text{C)}$$

$$\text{Temperature IPTS-68} = 1/[a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]] - 273.15 \text{ (}^\circ\text{C)}$$
Following the recommendation of JPOTS: T_{68} is assumed to be $1.00024 * T_{90}$ (-2 to 35 $^\circ\text{C}$)

Residual = instrument temperature - bath temperature

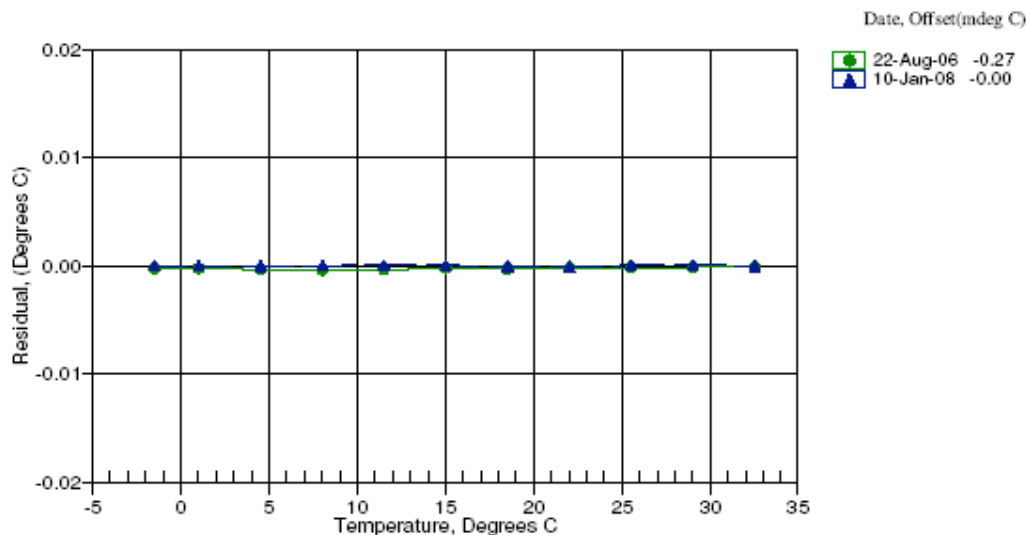

**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Temperature Calibration Report

Customer:	Raytheon Polar Services Co.		
Job Number:	48653	Date of Report:	1/10/2008
Model Number:	SBE 03Plus	Serial Number:	03P2308

Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.

'AS RECEIVED CALIBRATION'☒ **Performed** ☐ **Not Performed**

Date: 1/10/2008

Drift since last cal: +0.00019 Degrees Celsius/year

Comments:

'CALIBRATION AFTER REPAIR'☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: Degrees Celsius/year

Comments:

CTD Primary Conductivity Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1852
CALIBRATION DATE: 10-Jan-08SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHJ COEFFICIENTS


$g = -3.96023791e+000$
 $h = 5.05695912e-001$
 $i = -5.54651278e-004$
 $j = 5.41198276e-005$
 $CP_{cor} = -9.5700e-008$ (nominal)
 $CT_{cor} = 3.2500e-006$ (nominal)

ABCDM COEFFICIENTS

$a = 1.34913219e-006$
 $b = 5.03785467e-001$
 $c = -3.95422179e+000$
 $d = -8.58070150e-005$
 $m = 5.1$
 $CP_{cor} = -9.5700e-008$ (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.80157	0.00000	0.00000
-1.0000	34.9569	2.81484	7.97604	2.81484	0.00000
1.0000	34.9569	2.98683	8.18637	2.98684	0.00001
15.0000	34.9578	4.28713	9.62657	4.28709	-0.00004
18.5000	34.9569	4.63500	9.97607	4.63502	0.00002
29.0001	34.9510	5.72190	10.99480	5.72194	0.00004
32.5000	34.9401	6.09513	11.32281	6.09510	-0.00003

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / (10(1 + \delta t + \epsilon p)) \text{ Siemens/meter}$$
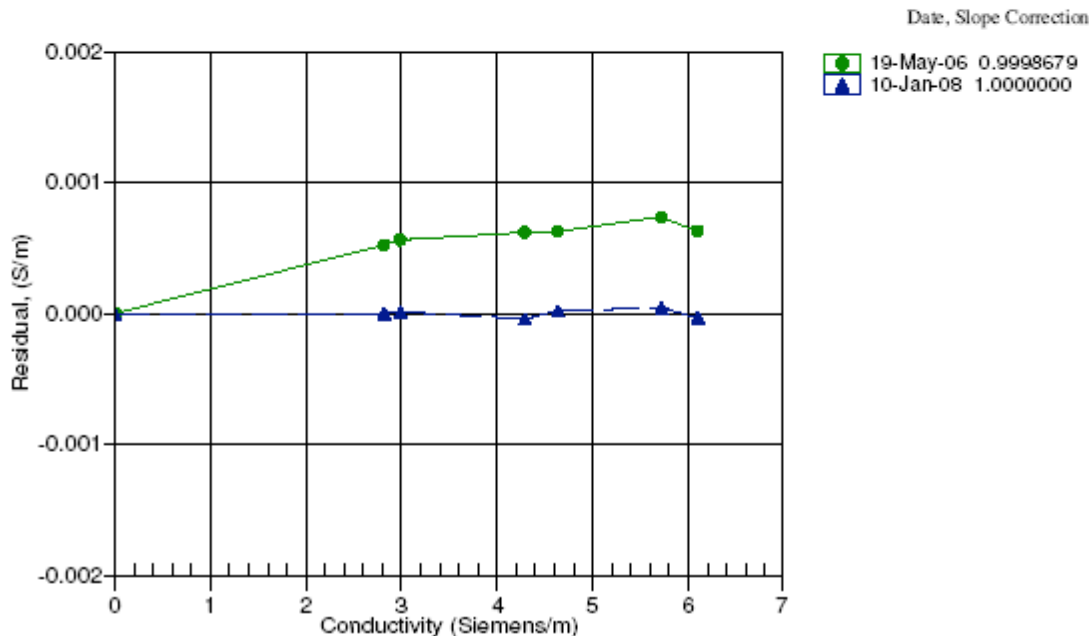
$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10(1 + \epsilon p)] \text{ Siemens/meter}$$
 $t = \text{temperature}[^{\circ}\text{C}]; p = \text{pressure}[\text{decibars}]; \delta = CT_{cor}; \epsilon = CP_{cor};$
 $\text{Residual} = (\text{instrument conductivity} - \text{bath conductivity}) \text{ using } g, h, i, j \text{ coefficients}$


**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Conductivity Calibration Report

Customer:	Raytheon Polar Services Co.		
Job Number:	48654	Date of Report:	1/10/2008
Model Number:	SBE 04C	Serial Number:	041852

Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.

'AS RECEIVED CALIBRATION'☒ **Performed** ☐ **Not Performed**

Date: 1/10/2008

Drift since last cal: -0.00020 PSU/month*

Comments:

'CALIBRATION AFTER CLEANING & REPLATINIZING'☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: PSU/month*

Comments:

*Measured at 3.0 S/m

Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.

CTD Secondary Conductivity Senesor (cast 001 -006)

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1850

CALIBRATION DATE: 26-Jun-07

SBE4 CONDUCTIVITY CALIBRATION DATA

PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHJ COEFFICIENTS

g = -4.34346018e+000

h = 5.22284785e-001

i = 8.35673592e-005

j = 2.23102434e-005

CPcor = -9.5700e-008 (nominal)

CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 4.56237821e-005

b = 5.22463069e-001

c = -4.34399624e+000

d = -8.41199524e-005

m = 3.8

CPcor = -9.5700e-008 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.88261	0.00000	0.00000
-1.0002	34.9338	2.81314	7.86998	2.81315	0.00001
0.9999	34.9342	2.98507	8.07497	2.98510	0.00002
14.9999	34.9346	4.28458	9.48007	4.28445	-0.00013
18.4999	34.9334	4.63221	9.82165	4.63227	0.00005
28.9999	34.9290	5.71868	10.81828	5.71883	0.00014
32.4999	34.9217	6.09227	11.13976	6.09217	-0.00010

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / [10(1 + \delta t + \epsilon p)] \text{ Siemens/meter}$$

$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10(1 + \epsilon p)] \text{ Siemens/meter}$$
t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correcti

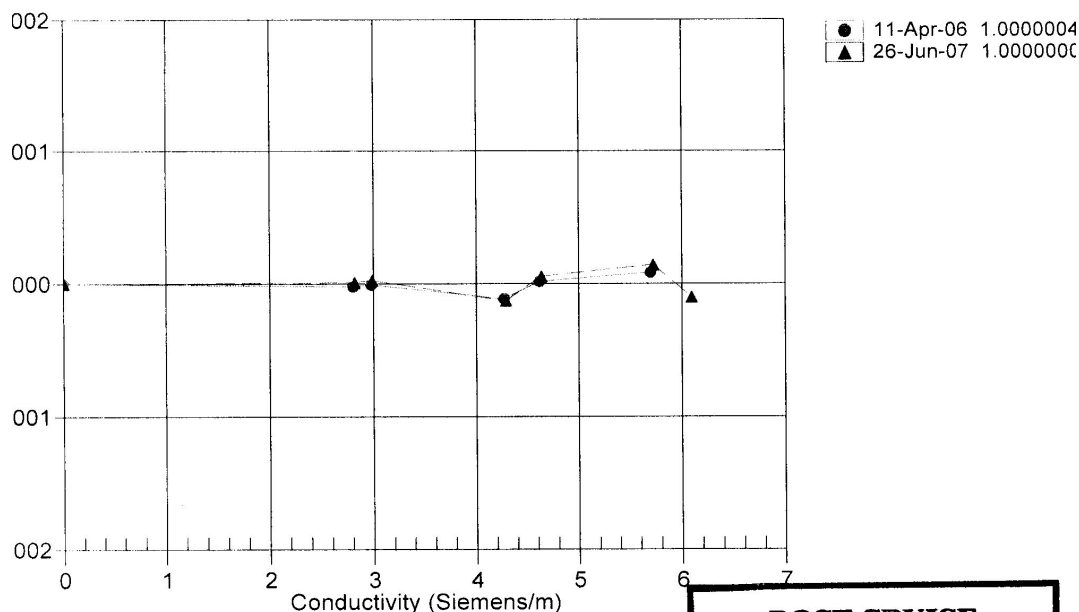
**POST CRUISE
CALIBRATION**

CTD Secondary Conductivity Senesor (cast 007 – on)

SEA-BIRD ELECTRONICS, INC.
 1808 136th Place N.E., Bellevue, Washington, 98005 USA
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1314
 CALIBRATION DATE: 08-Feb-08

SBE4 CONDUCTIVITY CALIBRATION DATA
 PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHI COEFFICIENTS

g = -4.07432471e+000
 h = 4.70852950e-001
 i = -3.55317882e-005
 j = 2.78698286e-005
 CPcor = -9.5700e-008 (nominal)
 CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 2.57454097e-005
 b = 4.70693911e-001
 c = -4.07357148e+000
 d = -7.95977201e-005
 m = 4.0
 CPcor = -9.5700e-008 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.94118	0.00000	0.00000
-1.0000	34.9363	2.81334	8.25650	2.81332	-0.00002
1.0000	34.9359	2.98521	8.47318	2.98524	0.00003
15.0000	34.9369	4.28484	9.95748	4.28482	-0.00002
18.5000	34.9367	4.63261	10.31787	4.63260	-0.00001
29.0001	34.9319	5.71913	11.36885	5.71917	0.00005
32.5000	34.9226	6.09242	11.70754	6.09239	-0.00003

Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

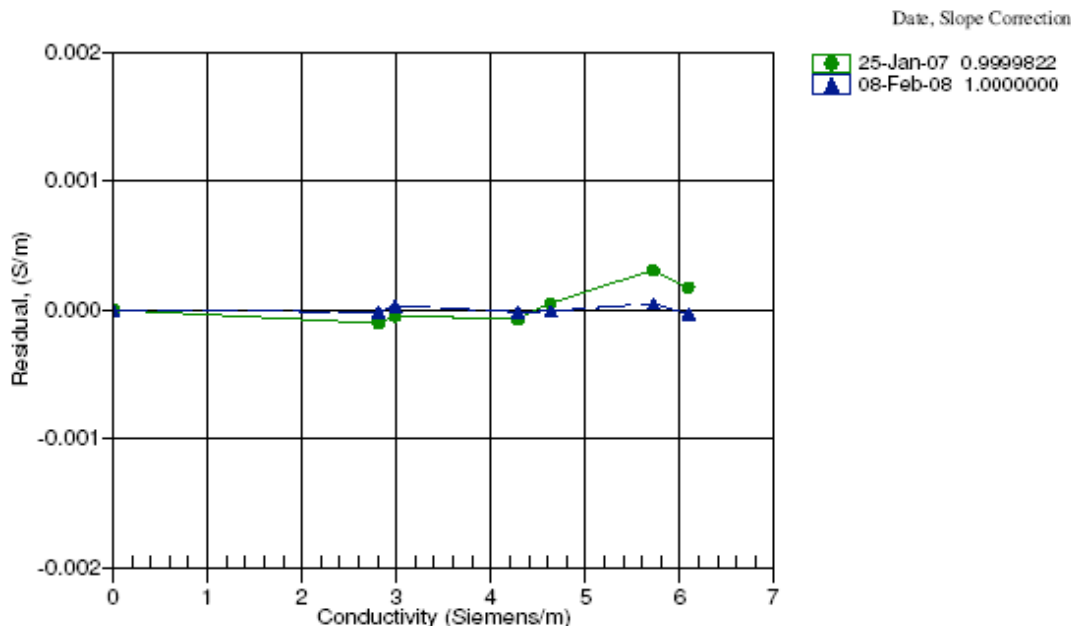

**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Conductivity Calibration Report

Customer:	Raytheon Polar Services Co.		
Job Number:	49000	Date of Report:	2/8/2008
Model Number:	SBE 04-02/0	Serial Number:	041314

Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.

'AS RECEIVED CALIBRATION'☒ **Performed** ☐ **Not Performed**

Date: 2/8/2008

Drift since last cal: 0.0000 PSU/month*

Comments:

'CALIBRATION AFTER CLEANING & REPLATINIZING'☐ **Performed** ☒ **Not Performed**

Date:

Drift since Last cal: PSU/month*

Comments:

**Measured at 3.0 S/m*

Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.

CTD Primary Dissolved Oxygen Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0082
CALIBRATION DATE: 09-Jan-08p

SBE43 OXYGEN CALIBRATION DATA

COEFFICIENTS

Soc = 0.2920

Boc = 0.0000

Voffset = -0.6150

TCor = 0.0008


PCor = 1.350e-04

BATH OX (m/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(m/l)	RESIDUAL (m/l)
1.23	20.00	0.01	1.271	1.24	0.01
1.24	26.00	0.01	1.347	1.24	0.00
1.24	12.00	0.01	1.176	1.25	0.01
1.24	2.00	0.00	1.053	1.24	-0.00
1.24	6.00	0.00	1.104	1.25	0.00
1.26	30.00	0.02	1.413	1.26	-0.00
4.09	20.00	0.01	2.792	4.11	0.01
4.11	26.00	0.01	3.041	4.10	-0.00
4.12	12.00	0.01	2.479	4.14	0.02
4.14	6.00	0.00	2.239	4.15	0.00
4.15	30.00	0.02	3.231	4.13	-0.01
4.16	2.00	0.00	2.078	4.14	-0.03
6.65	26.00	0.01	4.544	6.64	-0.01
6.67	30.00	0.02	4.830	6.66	-0.01
6.69	20.00	0.01	4.173	6.71	0.02
6.76	12.00	0.01	3.673	6.79	0.03
6.82	6.00	0.00	3.292	6.84	0.01
6.85	2.00	0.00	3.027	6.82	-0.03

$$\text{oxygen (m/l)} = (\text{Soc} * (\text{V} + \text{Voffset})) * \exp(\text{TCor} * \text{T}) * \text{Oxsat}(\text{T}, \text{S}) * \exp(\text{PCor} * \text{P})$$

V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU]

Oxsat(T,S) = oxygen saturation [m/l], P = pressure [dbar], Residual = instrument oxygen - bath oxygen

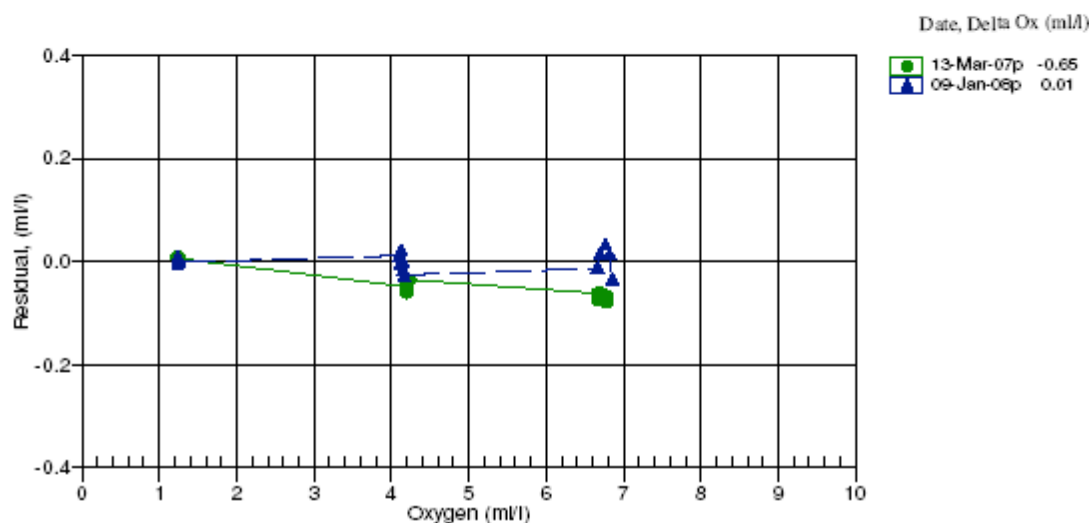

CTD Secondary Dissolved Oxygen Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0080
CALIBRATION DATE: 25-Jul-07p**SBE 43 OXYGEN CALIBRATION DATA****COEFFICIENTS**

Soc = 0.3584

Boc = 0.0000

Voffset = -0.5056

TCor = 0.0018

PCor = 1.350e-04

BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.25	30.00	0.01	1.126	1.24	-0.01
1.25	20.00	0.01	1.050	1.28	0.03
1.25	26.00	0.01	1.098	1.26	0.01
1.25	2.00	0.00	0.862	1.24	-0.02
1.25	12.00	0.01	0.973	1.29	0.04
1.25	6.00	0.00	0.907	1.27	0.01
4.09	30.00	0.01	2.518	4.02	-0.07
4.10	20.00	0.01	2.276	4.18	0.07
4.11	26.00	0.01	2.436	4.10	-0.01
4.13	12.00	0.01	2.033	4.21	0.09
4.15	6.00	0.00	1.825	4.16	0.01
4.15	2.00	0.00	1.673	4.06	-0.09
6.47	30.00	0.01	3.692	6.36	-0.12
6.50	26.00	0.01	3.552	6.48	-0.02
6.54	20.00	0.01	3.324	6.65	0.11
6.62	6.00	0.00	2.609	6.63	0.01
6.62	12.00	0.01	2.955	6.76	0.14
6.64	2.00	0.00	2.373	6.49	-0.14

$$\text{oxygen (ml/l)} = (\text{Soc} * (\text{V} + \text{Voffset})) * \exp(\text{TCor} * \text{T}) * \text{Oxsat}(\text{T}, \text{S}) * \exp(\text{PCor} * \text{P})$$


V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU]

Oxsat(T,S) = oxygen saturation [ml/l], P = pressure [dbar]

Residual = instrument oxygen - bath oxygen

Date, Delta Ox (ml/l)

● 17-Aug-06p 0.37
▲ 25-Jul-07p 0.03

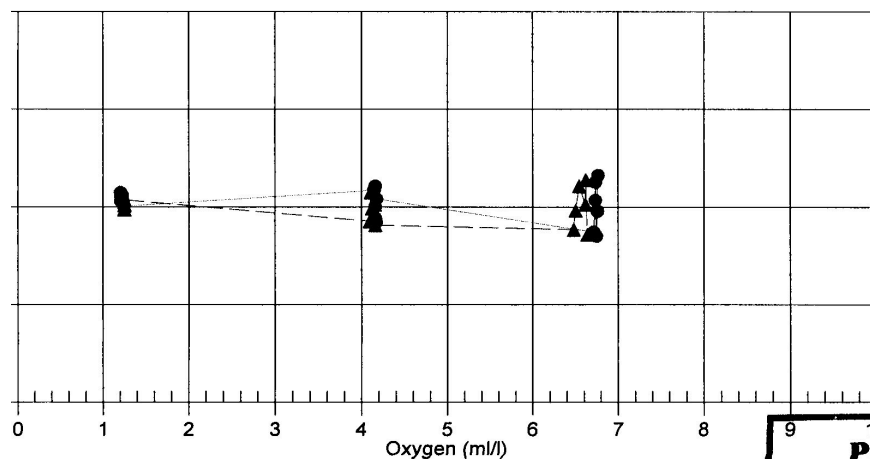

**POST CRUISE
CALIBRATION**

CTD Fluorometer

PO Box 518
620 Applegate St.
Philomath OR 97370



(541) 929-5650
Fax (541) 929-5277
<http://www.wetlabs.com>

Chlorophyll Fluorometer Characterization

Date: 10/16/06
Serial #: AFL-016D
Job#: 0102007
Tech: K.C

Dark Counts 0.221 volts
CEV 2.643 volts
SF 10.3220

FSV 5.45 volts

Linearity: 0.999 R² (0–1.5 volts)
0.995 R² (0– 5.45 volts)

Notes:

Dark Counts: Signal output of the meter in clean water with black tape over detector.

CEV is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to 25 µg/l of a *Thalassiosira weissflogii* phytoplankton culture.

SF is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determined by using the following equation:
 $SF = (25) / (CEV - \text{dark})$ e.g. $(25 / (2.865 - 0.238)) = 9.516$

FSV is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m³) can be derived by using the following equation: (µg/l) = $(V_{\text{measured}} - \text{dark}) * SF$

The relationship between fluorescence and chlorophyll-*a* concentrations in-situ is highly variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

CTD Transmissometer

PO Box 518
620 Applegate St.
Philomath, OR 97370



(541) 929-5650
Fax (541) 929-5277
www.wetlabs.com

C-Star Calibration

Date	July 27, 2007	Customer	National Science Foundation	Work order	002
Job #	0507014	S/N#	CST-889DR	Pathlength	25 cm

	Analog meter
V_d	0.060 V
V_{air}	4.837 V
V_{ref}	4.727 V

Temperature of calibration water	24.8 °C
Ambient temperature during calibration	26.1 °C

Relationship of transmittance (Tr) to beam attenuation coefficient (c), and pathlength (x): $Tr = e^{-cx}$

To determine beam transmittance: $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient: $c = -1/x * \ln(Tr)$

V_d Meter output with the beam blocked. This is the offset.

V_{air} Meter output in air with a clear beam path.

V_{ref} Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain V_{ref} .

Ambient temperature: meter temperature in air during the calibration.

V_{sig} Measured signal output of meter.

Revision G

3/5/07

MOCNESS***Mocness Temperature Sensor*****SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Temperature Calibration Report

Customer:	Raytheon Polar Services Co.		
Job Number:	39443	Date of Report:	6/13/2005
Model Number:	SBE 03Slow	Serial Number:	034080

Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.

'AS RECEIVED CALIBRATION'☒ Performed ☐ Not Performed

Date: 6/11/2005

Drift since last cal: +.00067 Degrees Celsius/year

Comments:

'CALIBRATION AFTER REPAIR'☐ Performed ☒ Not Performed

Date:

Drift since Last cal: Degrees Celsius/year

Comments:

Mocness Conductivity Sensor**SEA-BIRD ELECTRONICS, INC.**

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1431
CALIBRATION DATE: 10-Jan-08SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHIJ COEFFICIENTS

g = -4.25013133e+000

h = 5.51575692e-001

i = -1.35418342e-004

j = 3.71897020e-005

CPcor = -9.5700e-008 (nominal)

CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 1.71444628e-005

b = 5.51193302e-001

c = -4.24910323e+000

d = -8.43680316e-005


m = 4.2

CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.77609	0.00000	0.00000
-1.0000	34.9569	2.81484	7.65610	2.81481	-0.00004
1.0000	34.9569	2.98683	7.85618	2.98688	0.00004
15.0000	34.9578	4.28713	9.22704	4.28711	-0.00001
18.5000	34.9569	4.63500	9.56001	4.63500	0.00000
29.0001	34.9510	5.72190	10.53139	5.72191	0.00001
32.5000	34.9401	6.09513	10.84442	6.09512	-0.00001

Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meterConductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/metert = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

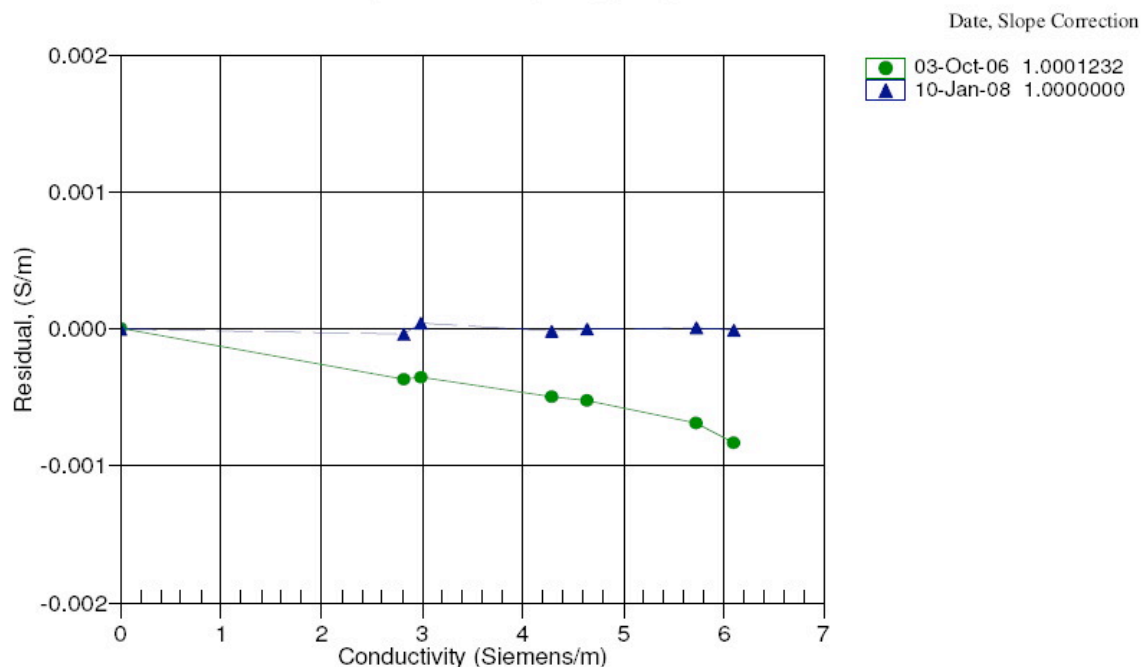

**SEA-BIRD ELECTRONICS, INC.**

1808 - 136th Place Northeast, Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Conductivity Calibration Report

Customer:	Raytheon Polar Services Co.		
Job Number:	48654	Date of Report:	1/10/2008
Model Number	SBE 04	Serial Number:	041431

Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.

'AS RECEIVED CALIBRATION'☒ Performed ☐ Not Performed

Date: 1/10/2008

Drift since last cal: +0.00020 PSU/month*

Comments:

'CALIBRATION AFTER CLEANING & REPLATINIZING'☐ Performed ☒ Not Performed

Date:

Drift since Last cal: PSU/month*

Comments:

**Measured at 3.0 S/m*

Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.

Mocness Fluorometer Sensor

PO Box 518
620 Applegate St.
Philomath OR 97370



(541) 929-5650
Fax (541) 929-5277
<http://www.wetlabs.com>

Chlorophyll Fluorometer Characterization ,Upon arrival at Wet Labs.

Date: 06/11/07
Serial #: AFLD-011
Job#: 0011007
Tech: K.C

Dark Counts 0.200 volts
CEV 2.654 volts
SF 10.1874

FSV 5.45 volts

Linearity: 0.999 R² (0–1.5 volts)
0.995 R² (0– 5.45 volts)

Notes:

Dark Counts: Signal output of the meter in clean water with black tape over detector.

CEV is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to 25 µg/l of a *Thalassiosira weissflogii* phytoplankton culture.

SF is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determine by using the following equation:
SF = (25) / (CEV – dark) e.g.(25 / (2.865 – 0.238) = 9.516)

FSV is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m³) can be derived by using the following equation: (µg/l) = (V_{measured} -dark) * SF

The relationship between fluorescence and chlorophyll-*a* concentrations in-situ is high variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

PO Box 518
620 Applegate St.
Philomath OR 97370



(541) 929-5650
Fax (541) 929-5277
<http://www.wetlabs.com>

Chlorophyll Fluorometer Characterization .

Date: 06/18/07
Serial #: AFLD-011
Job#: 0011007
Tech: K.C

Dark Counts 0.171 volts
CEV 2.660 volts
SF 10.0441

FSV 5.45 volts

Linearity: 0.999 R² (0-1.5 volts)
0.995 R² (0-5.45 volts)

Notes:

Dark Counts: Signal output of the meter in clean water with black tape over detector.

CEV is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to 25 µg/l of a *Thalassiosira weissflogii* phytoplankton culture.

SF is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determined by using the following equation:
SF = (25) / (CEV - dark) e.g. (25 / (2.865 - 0.238) = 9.516)


FSV is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m³) can be derived by using the following equation: (µg/l) = (V_{measured} - dark) * SF

The relationship between fluorescence and chlorophyll-*a* concentrations in-situ is highly variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

Mocness Transmissometer Sensor

PO Box 518
620 Applegate St.
Philomath, OR 97370



(541) 929-5650
Fax (541) 929-5277
www.wetlabs.com

C-Star Calibration

Date November 14, 2007 S/N# CST-439DR Pathlength 25 cm

	Analog meter
V_d	0.060 V
V_{air}	4.794 V
V_{ref}	4.683 V

Temperature of calibration water	23.2 °C
Ambient temperature during calibration	25.9 °C

Relationship of transmittance (Tr) to beam attenuation coefficient (c), and pathlength (x): $Tr = e^{-cx}$

To determine beam transmittance: $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient: $c = -1/x * \ln(Tr)$

V_d Meter output with the beam blocked. This is the offset.

V_{air} Meter output in air with a clear beam path.

V_{ref} Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain V_{ref} .

Ambient temperature: meter temperature in air during the calibration.

V_{sig} Measured signal output of meter.