


# Data Report NBP1001

Antarctic Peninsula

Dr. Eugene Domack

4 January to 1 March 2010

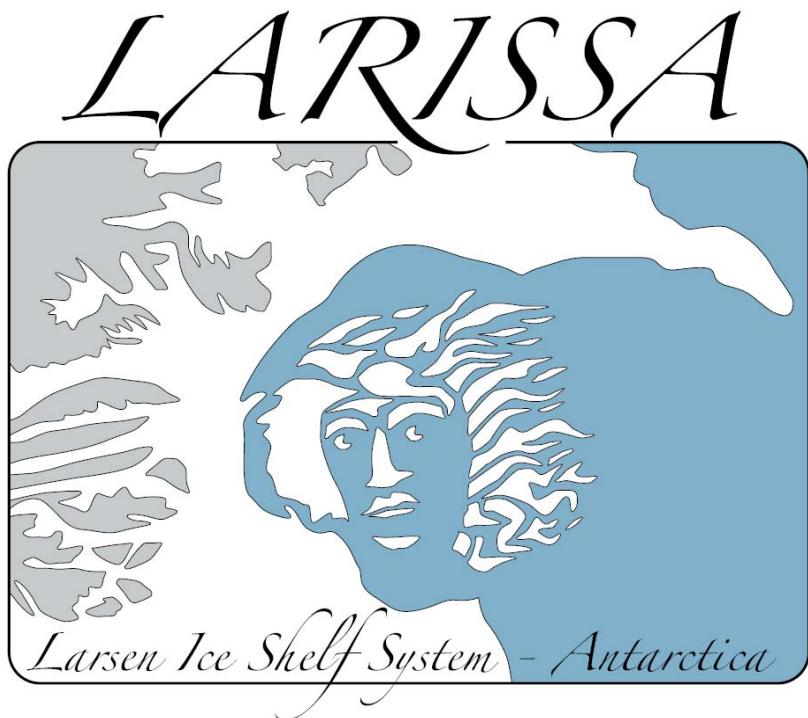

RVIB Nathaniel B. Palmer

United States Antarctic Program

Raytheon Polar Services Corporation

Prepared by Paul Huckins and Dmitriy Tizon

## Table of Contents

<b>INTRODUCTION.....</b>	<b>1</b>
NBP1001 DISTRIBUTION SPECIFICS.....	2
<b>DISTRIBUTION CONTENTS AT A GLANCE.....</b>	<b>3</b>
EXTRACTING DATA.....	5
<b>DISTRIBUTION CONTENTS .....</b>	<b>6</b>
CRUISE INFORMATION .....	6
CRUISE TRACK.....	6
SATELLITE IMAGES .....	6
NBP DATA PRODUCTS.....	6
<i>JGOFS</i> .....	7
<i>MGD77</i> .....	8
SCIENCE OF OPPORTUNITY .....	9
<i>ADCP</i> .....	9
<i>pCO<sub>2</sub></i> .....	9
CRUISE SCIENCE .....	10
<i>CTD</i> .....	10
RVDAS .....	10
<i>Sensors and Instruments</i> .....	10
Underway Sensors .....	11
Meteorology and Radiometry.....	11
Geophysics .....	11
Oceanography.....	11
Navigational Instruments.....	12
Data.....	12
Underway Data .....	13
Sound Velocity Probe (svp1).....	13
Meteorology (mwx1).....	13
MET string .....	13
PUS string .....	14
SUS string .....	14
Knudsen (knud).....	14
Fluorometer (flr1).....	14
pCO <sub>2</sub> (pco2).....	15
Simrad EM120 (mbdp).....	15
Micro-TSG (mtsg).....	15
Gravimeter (grv1).....	16
Engineering (eng1).....	17
Hydro-DAS (hdas) .....	18
GUV Data (pguv).....	18
Remote Temperature (rtmp) .....	18
Navigational Data .....	19
Seapath GPS (seap) .....	19
Trimble (P-Code) GPS (PCOD) .....	21
Gyro Compass (gyr1) .....	22
ADCP Course (adcp) .....	22
Processed Data.....	23
pCO <sub>2</sub> -merged .....	23
<b>CALCULATIONS .....</b>	<b>24</b>
PAR.....	24
PSP.....	24
PIR .....	25
<b>ACQUISITION PROBLEMS AND EVENTS.....</b>	<b>26</b>

<b>APPENDIX: SENSORS AND CALIBRATIONS .....</b>	<b>27</b>
<i>NBP1001 Shipboard Sensors .....</i>	27
Meteorology & Radiometers .....	27
Underway .....	27
<i>NBP1001 CTD Sensors .....</i>	28
CALIBRATIONS.....	28
<i>Gravity Tie Start (Punta Arenas) .....</i>	29
<i>Barometer.....</i>	30
<i>Humidity Sensor.....</i>	31
<i>Wet Temperature (part of humidity) Sensor.....</i>	32
<i>PIR .....</i>	33
<i>PSP.....</i>	34
<i>Mast PAR .....</i>	35
<i>GUV (Mast).....</i>	36
<i>Remote Temperature (Primary) .....</i>	39
<i>Remote Temperature (Secondary).....</i>	40
<i>Underway fluorometer .....</i>	41
<i>Underway Transmissometer.....</i>	42
<i>CTD Fish &amp; Pressure Sensor.....</i>	43
<i>CTD Conductivity (Primary).....</i>	44
<i>CTD Conductivity (Secondary).....</i>	45
<i>CTD Temperature (Primary) .....</i>	46
<i>CTD Temperature (Secondary).....</i>	47
<i>CTD Pump (Primary).....</i>	48
<i>CTD Pump (Secondary) .....</i>	49
<i>CTD Dissolved Oxygen (Primary) .....</i>	50
<i>CTD Dissolved Oxygen (Secondary).....</i>	51
<i>CTD Fluorometer.....</i>	52
<i>CTD Transmissometer .....</i>	53
<i>CTD PAR.....</i>	54

## Introduction

The NBP data acquisition systems continuously log data from the instruments used during the cruise. This document describes:

- The structure and organization of the data on the distribution media
- The format and contents of the data strings
- Formulas for calculating values
- Information about the specific instruments in use during the cruise
- A log of acquisition problems and events during the cruise that may affect the data
- Scanned calibration sheets for the instruments in use during the cruise.

The data is distributed on a DVD-R or CD-ROM written in ISO9660 level-1 format. It is readable by virtually every computing platform. (see next section ‘NBP1001 Distribution Set’ for details specific to that data)

All the data has been compressed using Unix “gzip,” identified by the “.gz” extension. It has been copied to the distribution media in the Unix tar archive format, “.tar” extension. Tools are available on all platforms for uncompressing and de-archiving these formats: On Macintosh, use Stuffit Expander with DropStuff. On Windows operating systems use WinZip.

MultiBeam data is distributed separately and not covered in this report.

Raw ADCP data can be obtained from Eric Firing at the University of Hawaii.

*IMPORTANT: Read the last section, “Acquisition Problems and Events,” for important information that may affect the processing of this data.*

## NBP1001 Distribution Specifics

The NBP1001 data set was larger than most. The complete, data set, consists of 14 DVDs.

<b>Basic Data set</b>	
All DAS	Primary DVD
All CTD	Primary DVD
Imagery	Primary DVD
Sidescan	Second DVD
Watch	Second DVD
e-log	Second DVD
LADCP	Second DVD
Mooring	Second DVD
Nutrients	Second DVD

<b>Additional Data Sets</b>	
Bathy 2kw	2 DVDs
Knudsen	2 DVDs
YoYo Cam	4 DVDs
MegaCore Video	4 DVDs
EK_500	1 DVD

This data report only fully describes the data on disk 1 of the ‘Basic Data Set.’ Disk 1 of the ‘Basic Data Set’ is written in ISO9660 level-1 format.

All other disks are written in Joliet extended format and the ISO9660 characterset. These disks should all be readable on any recent Windows, Macintosh, or Linux computer platforms.

None of the data on the ‘additional disks’ has been compressed. There is no uncompression software needed.

We make no attempt to describe in detail the additional data sets. We provide only the following general details for this data.

**Bathy 2000W** data is SEG-Y data that was collected with a ODEC Bathy 2000 and processed using InterActive Oceanographics Bathy 2000W for Windows software.

**Knudsen** data was collected with a Knudsen 320 B/R and playback software is available from Kundsen

**EK 500** data was collected with a Simrad EK500 and processed with Myriax ‘echoview’ software. Their software is available at [www.myriax.com](http://www.myriax.com)

**YoYoCam** files are in standard jpeg format and should be easily readable on almost any computer.

**MegaCore** Videos are in standard .avi format and should be easily readable on almost any computer. Still shots are standard .png formats.

## Distribution Contents at a Glance

### Basic Data Set

#### Volume 1 of 2: NBP1001

File	Description
/	Root level directory
NBP1001.trk	Text file of cruise track (lat,lon)
NBP1001.mgd	Full Cruise MGD77 data file
NBP1001.gmt	GMT binary file of MGD77 data
INSTCOEF.TXT	Instrument Coefficient File
1001DATA.doc	Data Report NBP1001 (MS Word)
1001DATA.pdf	Data Report NBP1001 (pdf)
1001MBReport.doc	Multibeam Report (MS Word)
1001_trak.ps	Cruise track plot (PostScript format)
1001_trak.jpg	Cruise track plot (JPEG format)
/process	Processed data
1001jgof.tar	JGOFS format data files
1001qc.tar	Daily RVDAS QC postscript plots
1001pco2.tar	Merged pCO2 data files
1001mgd.tar	MGD Data
1001proc.tar	Other processed data
/rvdas/nav	Navigation data
1001gyr1.tar	Gyro raw data
1001pcod.tar	Trimble P-code raw data
1001seap.tar	Seapath data
1001adcps.tar	ADCP Data Sets
/rvdas/uw	Underway data
1001bat1.tar	Bathy 2000 data
1001eng1.tar	Engineering Data
1001grv1.tar	Gravimeter raw data
1001hdas.tar	HydroDAS raw data
1001knud.tar	Knudsen raw data
1001mbdp.tar	MulitBeam Center depth data
1001mtsg.tar	Micro TSG data
1001mwx1.tar	Meteorology raw data
1001pco2.tar	pCO2 raw data
1001pguv.tar	GUV raw data
1001rtmp.tar	Remote temperature data
1001sim1.tar	Simrad EK500 data
1001svp1.tar	Sound velocity probe (in ADCP well)
/Imagery	Other data, files and pictures
1001lImag.tar	Satellite imagery
/ocean	Ocean data
1001ctd.tar	CTD Data
1001xbt.tar	XBT Data

<b>Basic Data Set</b>	
<b>Volume 2 of 2: NBP1001</b>	
<b>File</b>	<b>Description</b>
/ CTD_LADCP elog_backup Moorings Nutrients side scan files watch files	<p>Root level directory</p> <p>This data is not described in detail in this report. It is included to as a convenience to the science party.</p>

## Extracting Data

The Unix tar command has many options. It is often useful to know exactly how an archive was produced when expanding its contents. All archives were created using the command,

```
tar cvf archive_filename files_to_archive
```

To create a list of the files in the archive, use the Unix command,

```
tar tvf archive_filename > contents.list
```

where contents.list is the name of the file to create

To extract the files from the archive:

```
tar xvf archive_filename file(s)_to_extract
```

G-zipped files will have a “.gz” extension on the filename. These files can be decompressed after de-archiving, using the Unix command,

```
gunzip filename.gz
```

## Distribution Contents

### Cruise Information

NBP1001 departed Punta Arenas, Chile on January 4<sup>th</sup> 2010. There were various unscheduled stops during the cruise. Three at Palmer Station, one at Rothera Base. The sea state was good but low clouds kept visibility down. Much of the science depended on using helicopters to deposit equipment and work teams to various field sites. The lack of visibility was a big factor during much of the cruise. We did not have current permits to collect data in Argentine waters on the transit south. Data collection was started as we left the Argentine EEZ and crossed into international waters. Our permits were in order for the transit north. Data collection for LARISSA was stopped GMT 23:59 on Julian day 057. Additional jgofs data was collected for the science of opportunity experiments, until such time as we crossed into the Chilean EEZ. The NBP returned to Punta Arenas on March 1<sup>st</sup> 2010. There is a separate distribution with Argentine data only.

### Cruise Track

The distribution DVD includes a GMT cruise track file (NBP1001.trk). It contains the longitude and latitude of the ship's position at one-minute intervals extracted from the NBP1001.gmt file. JPEG and PostScript cruise track files have been produced and placed in the /plots directory.

### Satellite Images

Satellite Images received for this cruise can be found in the file called /Imagery/1001Imag.tar collected and processed on the ship is in two further subdirectories, Ice and WX (weather). Files are named using the convention, ssss\_fff\_mmmddyy\_tttt\_ww.gif where:

ssss\_fff = satellite and flight number  
mm = month  
dd = day  
yy = year  
tttt = time in hours and minutes (UTC)  
ww = optional field for identifying wavelength, such as vis (visible) or IR (infrared)

### NBP Data Products

Two datasets are created on each cruise: JGOFS and MGD77.

The data processing scripts used to produce JGOFS and MGD77 data sets create a lot of intermediate files. These files are included on the data distribution media in a file called /process/1001proc.tar. They are included to make re-processing easier in the event of an error, but no extensive detail of the formats is included in this document. If you have any questions, please contact [itvessel@usap.gov](mailto:itvessel@usap.gov).

## JGOFS

The JGOFS data set can be found on the distribution media in the file /process/1001jgof.tar. The archive contains one file produced for each day named jgDDD.dat.gz, where DDD is the year-day the data was acquired. The ".gz" extension indicates that the individual files are compressed before archiving. Each daily file consists of 22 columnar fields in text format as described in the table below. The JGOFS data set is created from calibrated data decimated at one-minute intervals. Several fields are derived measurements from more than a single raw input. For example, Course Made Good (CMG) and Speed Over Ground (SOG) are calculated from gyro and GPS inputs. Daily plots during the cruise are produced from the JGOFS data set. Note: Null, unused, or unknown fields are indicated as "NAN" as 9999 in the JGOFS data.

Field	Data	Units
01	GMT date	dd/mm/yy
02	GMT time	hh:mm:ss
03	NGL latitude (negative is South)	tt.tttt
04	NGL longitude (negative is West)	ggg.gggg
05	Speed over ground	Knots
06	GPS HDOP	-
07	Gyro Heading	Degrees (azimuth)
08	Course made good	Degrees (azimuth)
09	Mast PAR	$\mu$ Einstens/meter <sup>2</sup> sec
10	Sea surface temperature	°C
11	Sea surface conductivity	siemens/meter
12	Sea surface salinity	PSU
13	Sea depth (uncorrected, calc. sw sound vel. 1500 m/s)	meters
14	True wind speed (max speed windbird)	meters/sec
15	True wind direction (max speed windbird)	degrees (azimuth)
16	Ambient air temperature	°C
17	Relative humidity	%
18	Barometric pressure	mBars
19	Sea surface fluorometry	$\mu$ g/l (mg/m <sup>3</sup> )
20	Transmissometry	%
21	PSP	W/m <sup>2</sup>
22	PIR	W/m <sup>2</sup>

## MGD77

The MGD77 data set is contained in a single file for the entire cruise. It can be found in the top level of the distribution data structure as NBP1001.mgd. The file NBP1001.gmt is created from the MGD77 dataset using the "mgd77togmt" utility. NBP1001.gmt can be used with the GMT plotting package.

The data used to produce the NBP1001.mgd file can be found on the distribution media in the file /process/1001proc.tar. The data files in the archive contain a day's data and follow the naming convention Dddd.fnl.gz, where ddd is the year-day. These files follow a space-delimited columnar format that may be more accessible for some purposes. They contain data at one-second intervals rather than one minute and are individually "gzipped" to save space. Below is a detailed description of the MGD77 data set format. The other files in the archive contain interim processing files and are included to simplify possible reprocessing of the data using the RVDAS NBP processing scripts.

All decimal points are implied. Leading zeros and blanks are equivalent. Unknown or unused fields are filled with 9's. All "corrections", such as time zone, diurnal magnetics, and EOTVOS, are understood to be added.

Col	Len	Type	Contents	Description, Possible Values, Notes
1	1	Int	Data record type	Set to "5" for data record
2-9	8	Char	Survey identifier	
10-12	3	int	Time zone correction	Corrects time (in characters 13-27) to GMT when added; 0 = GMT
13-16	4	int	Year	4 digit year
17-18	2	int	Month	2 digit month
19-20	2	int	Day	2 digit day
21-22	2	int	Hour	2 digit hour
23-27	5	real	Minutes x 1000	
28-35	8	real	Latitude x 100000	+ = North - = South. (-9000000 to 9000000)
36-44	9	real	Longitude x 100000	+ = East - = West. (-18000000 to 18000000)
45	1	int	Position type code	1=Observed fix 3=Interpolated 9=Unspecified
46-51	6	real	Bathymetry, 2- way travel time	In 10,000th of seconds. Corrected for transducer depth and other such corrections
52-57	6	real	Bathymetry, corrected depth	In tenths of meters.
58-59	2	int	Bathymetric correction code	This code details the procedure used for determining the sound velocity correction to depth
60	1	int	Bathymetric type code	1 = Observed 3 = Interpolated (Header Seq. 12) 9 = Unspecified
61-66	6	real	Magnetics total field, 1 <sup>st</sup> sensor	In tenths of nanoteslas (gammas)
67-72	6	real	Magnetics total field, 2 <sup>nd</sup> sensor	In tenths of nanoteslas (gammas), for trailing sensor
73-78	6	real	Magnetics residual field	In tenths of nanoteslas (gammas). The reference field used is in Header Seq. 13
79	1	int	Sensor for residual field	1 = 1 <sup>st</sup> or leading sensor 2 = 2 <sup>nd</sup> or trailing sensor 9 = Unspecified

Col	Len	Type	Contents	Description, Possible Values, Notes
80-84	5	real	Magnetics diurnal correction	In tenths of nanoteslas (gammas). (In nanoteslas) if 9-filled (i.e., set to "+9999"), total and residual fields are assumed to be uncorrected; if used, total and residuals are assumed to have been already corrected.
85-90	6	F6.0	Depth or altitude of magnetics sensor	(In meters) + = Below sea level 3 = Above sea level
91-97	7	real	Observed gravity	In 10 <sup>th</sup> of mgals. Corrected for Eotvos, drift, tares
98-103	6	real	EOTVOS correction	In 10 <sup>th</sup> of mgals. $E = 7.5 V \cos \phi \sin \alpha + 0.0042 V^* V$
104-108	5	real	Free-air anomaly	In 10 <sup>th</sup> of mgals G = observed G = theoretical
109-113	5	char	Seismic line number	Cross-reference for seismic data
114-119	6	char	Seismic shot-point number	
120	1	int	Quality code for navigation	5=Suspected, by the originating institution 6=Suspected, by the data center 9=No identifiable problem found

## Science of Opportunity

### ADCP

The shipboard ADCP system measures currents in a depth range from about 30 to 300 m -- in good weather. In bad weather or in ice, the range is reduced, and sometimes no valid measurements are made. ADCP data collection is the OPP-funded project of Eric Firing (University of Hawaii) and Teri Chereskin (Scripps Institution of Oceanography). Data is collected on both the LMG and the NBP for the benefit of scientists on individual cruises, and for the long-term goal of building a profile of current structure in the Southern Ocean.

A data feed is sent from the ADCP system to RVDAS whenever a reference layer is acquired. This feed contains east and north vectors for ship's speed, relative to the reference layer, and ship's heading. Collected files (one per day) are archived in 1001adcp.tar in the directory /rvdas/nav.

### pCO<sub>2</sub>

The NBP carries a pCO<sub>2</sub> measurement system from Lamont-Doherty Earth Observatory (LDEO). pCO<sub>2</sub> data is recorded by RVDAS and transmitted to LDEO at the end of each cruise. You will find pCO<sub>2</sub> data in a file named 1001pco2.tar in the /process directory, which contains the pCO<sub>2</sub> instrument's data merged with GPS, meteorological and other oceanographic measurements. For more information contact Colm Sweeney (csweeney@ldeo.columbia.edu).

## Cruise Science

### **CTD**

The ctd data has been placed in the tar file /ocean/1001ctd.tar. The archive contains tar files 1001proc.tar.

## RVDAS

The Research Vessel Data Acquisition System (RVDAS) was developed at Lamont-Doherty Earth Observatory of Columbia University and has been in use on its research ship for many years. It has been extensively adapted for use on the USAP research vessels.

Daily data processing of the RVDAS data is performed to calibrate and convert values into useable units and as a quality-control on operation of the DAS. Raw and processed data sets from RVDAS are included in the data distribution. The tables below provide detailed information on the sensors and data. Be sure to read the "Significant Acquisition Events" section for important information about data acquisition during this cruise.

### **Sensors and Instruments**

RVDAS data is divided into two general categories, *underway and navigation*. They can be found on the distribution media as subdirectories under the top level rvdas directory: /rvdas/uw, and /rvdas/nav. Processed oceanographic data is in the top level directory, /process. Each instrument or sensor produces a data file named with its channel ID. Each data file is g-zipped to save space on the distribution media. Not all data types are collected every day or on every cruise.

The naming convention for data files produced by the sensors and instruments is

NBP[CruiseID][ChannelID].dDDD

Example: NBP1001.mwx1.d330

- The CruiseID is the numeric name of the cruise, in this case, NBP1001.
- The ChannelID is a 4-character code representing the system being logged. An example is "mwx1," the designation for meteorology.
- DDD is the day of year the data was collected

## Underway Sensors

### Meteorology and Radiometry

Measurement	Channel ID	Collect. Status	Rate	Instrument
Air Temperature	mwx1	continuous	1 sec	R.M. Young 41372LC
Relative Humidity	mwx1	continuous	1 sec	R.M. Young 41372LC
Wind Speed/Direction	mwx1	continuous	1 sec	Gill 1390-PK-007
Barometer	mwx1	continuous	1 sec	R.M. Young 61201
PIR (LW radiation)	mwx1	continuous	1 sec	Eppley PIR
PSP (SW radiation)	mwx1	continuous	1 sec	Eppley PSP
PAR	mwx1	continuous	1 sec	BSI QSR-240
GUV	pguv	continuous	2 sec	BSI PUV-2511
PUV	pguv	not collected		BSI PUG-2500

### Geophysics

Measurement	Channel ID	Collect. Status	Rate	Instrument
Gravimeter	grv1	continuous	10 sec*	LaCoste & Romberg
Magnetometer	mag1	not collected	15 sec	EG&G G-866
Bathymetry	bat1	continuous**	Varies	ODEC Bathy 2000
Bathymetry	knud	continuous	Varies	Knudsen 320B/R
Bathymetry	sim1	not collected	Varies	Simrad EK500 Sonar

\*Data is output every second but it only changes every 10 seconds.

\*\*Primary underway bathymetry was switched from Knudsen to Bathy 2000 at 016:16:33.

### Oceanography

Measurement	Channel ID	Collect. Status	Rate	Instrument
Conductivity	mtsg	Continuous	6 sec	SeaBird SBE-45
Salinity	mtsg	Continuous	6 sec	Calc. from pri. temp
Sea Surface Temp	mtsg	Continuous	6 sec	SeaBird 3-01/S
Fluorometry	hdas	Continuous	2 sec	WET Lab AFL
Transmissometry	hdas	Continuous	2 sec	WET Lab C-Star
pCO <sub>2</sub>	Pco2	Continuous	70 sec	(LDEO)
ADCP	adcp	Continuous	varies	RD Instruments

## Navigational Instruments

Measurement	Channel ID	Collect. Status	Rate	Instrument
Trimble GPS	PCOD	Continuous	1 sec	Trimble 20636-00SM
Gyro	gyr1	Continuous	0.2 sec	Yokogawa Gyro
SeaPath	seap	Continuous	1 sec	SeaPath 200

### **Data**

Data is received from the RVDAS system via RS-232 serial connections. A time tag is added at the beginning of each line of data in the form,

```
yy+dd:hh:mm:ss.sss [data stream from instrument]
```

where

yy	= two-digit year
ddd	= day of year
hh	= 2 digit hour of the day
mm	= 2 digit minute
ss.sss	= seconds

All times are reported in UTC.

The delimiters that separate fields in the raw data files are often spaces and commas but can be other characters such as : = @. Occasionally no delimiter is present. Care should be taken when reprocessing the data that the field's separations are clearly understood.

In the sections below a sample data string is shown, followed by a table that lists the data contained in the string.

## **Underway Data**

Each section below describes a type of data file (file name extension in parentheses) followed by a typical line of data in the file. In the table(s) for each section is a description of the fields within each line of data. Note: most data files listed below will be included with each cruise's data distribution; however some types of files may be omitted if the instrument was not operating during the cruise. The available data files can be found in the /rvdas/uw directory on the distribution disc.

### **Sound Velocity Probe (svp1)**

08+330:00:00:49.011 1519.35

Field	Data	Units
1	RVDAS Time tag	
2	Sound velocity in ADCP sonar well	m/s

### **Meteorology (mwx1)**

There are 3 different data strings in the mwx1 data file:

MET

08+330:23:59:57.725 MET,12.1,-54,6.64,88.7,111.3374,0.02414567,-  
0.4827508,282.9581,281.8823,1003.119

PUS

08+330:23:59:58.546 PUS,A,020,008.53,M,+337.12,+009.00,00,0F

SUS

08+330:23:59:58.779 SUS,A,017,008.76,M,+335.53,+006.35,00,02

### **MET string**

Field	Data	Units
1	RVDAS time tag	
2	MET (string flag)	
3	Power Supply Voltage	V
4	Enclosure Relative Humidity	%
5	Air temperature	°C
6	Air Relative Humidity	%
7	PAR (photosynthetically available radiation)*	mV
8	PSP (short wave radiation)*	mV
9	PIR Thermopile (long wave radiation)*	mV
10	PIR Case Temperature	°Kelvin
11	PIR Dome Temperature	°Kelvin
12	Barometer	mBar

\*See page 21 for calculations.

**PUS string**

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	PUS (string flag)	
3	A (unit identification)	
4	Port Wind direction relative	deg
5	Port Wind speed relative	m/s
6	Units	
7	Sound Speed	m/s
8	Sonic Temperature	°C
9	Unit Status (00 or 60 are good, any other value indicates fault)	
10	Check Sum	

**SUS string**

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	SUS (string flag)	
3	A (unit identification)	
4	Starboard Wind direction relative	deg
5	Starboard Wind speed relative	m/s
6	Units	
7	Sound Speed	m/s
8	Sonic Temperature	°C
9	Unit Status (00 or 60 are good, any other value indicates fault)	
10	Check Sum	

**Knudsen (knud)**

99+099:00:18:19.775 HF,305.2,LF,304.3

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	HF = High frequency flag (12 kHz)	
3	High frequency depth	meters
4	LF = Low frequency flag (3.5 kHz)	
5	Low frequency depth	meters

**Fluorometer (flr1)**

This Fluorometer is not in use. Current Fluorometer goes to the hdas string.

00+019:23:59:58.061 0 0818 :: 1/19/00 17:23:17 = 0.983 (RAW) 1.2 (C)

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	Marker 0 to 8	
3	4-digit index	
4	Date	mm/dd/yy
5	Time	hh:mm:ss
6	Signal	
7	Signal units of measurement	
8	Cell temperature (if temperature compensation package is installed)	
9	Temperature units (if temperature compensation package is installed)	

**pCO<sub>2</sub> (pco2)**

00+021:23:59:43.190 2000021.99920 2382.4 984.2 30.73 50.8 345.9 334.1 -1.70  
 -68.046 -144.446 Equil

Field	Data	Units
1	RVDAS time tag	
2	pCO <sub>2</sub> time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temperature	°C
5	Barometer	MBar
6	Concentration	ppm
7	Equilibrated temperature	°C
8	pCO <sub>2</sub> pressure	microAtm
9	Flow rate	ml / min
10	Source ID #	1 or 2 digits
11	Valve position	1 or 2 digits
12	Flow source (Equil = pCO <sub>2</sub> measurement)	text

**Simrad EM120 (mbdp)**

09+282:10:53:38.318 \$KGDPT,3945.60,7.29,1;12000.0\*7c

Field	Data	Units
1	RVDAS time tag	
2	EM120 (string flag)	
3	Depth below keel	Meters
4	Keel depth	Meters
5		

**Micro-TSG (mtsg)**

08+330:23:59:40.894 5.9322, 3.34685, 34.0550, 1473.281

Field	Data	Units
1	RVDAS time tag	
2	Internal Temperature	°C
3	Conductivity	s/m
4	Salinity	PSU
5	Sound velocity	m/s

## Gravimeter (grv1)

There are now two sets of fields output by the gravity meter. The data record is output once per second, and identified by "\$DAT" in the id field. A summary of sensor environmental data is output every ten seconds, identified by "%ENV" in the id field.

### Data record (\$DAT):

05+194:00:00:27.995 \$DAT,2005/ 7/13, 0: 7: 7.36,194, 9050.37, 9050.06, 5410.86, -0.00, -0.01, -0.02, 0.00, 0.00, 0.70, 0.19, -0.12, -0.25, 0.00, -69.45711315, -54.32181487, 0.000, 285.200,

Field	Data	Conversion	Units
1	RVDAS time tag		
2	Text string (id field)	\$DAT for data record	
3	Date	YYYY/MM/DD	
4	Time	HH:MM:SS.SS	
5	Day of Year	DDD	
6	Gravity count	mgal = count x 1.0046 + offset	count
7	Spring Tension		CU
8	Beam Position	Volts x 750,000	
9	VCC		
10	AL		
11	AX		
12	VE		
13	AX2		
14	XACC2		
15	LACC2		
16	CROSS ACCEL		GAL
17	LONG ACCEL		GAL
18	EOTVOS CORR		MGAL
19	LONGITUDE		Degrees
20	LATITUDE		Degrees
21	HEADING		Degrees
22	VELOCITY		Knots

**Environmental record (\$ENV)**

05+183:19:13:10.945 %ENV,2005/ 7/ 2,19:19:52.16,183,S-036/V1.5, 3.34,  
 47.19, 20.34,1.111840E-1,-0.57700,-0.10591, 0.40180, 2.55260, 0.43000, 1,  
 300

Field	Data	Conversion	Units
1	RVDAS time tag		
2	Text string (id field)	\$ENV for environmental record	
3	Date	YYYY/MM/DD	
4	Time	HH:MM:SS.SS	
5	Day of Year	DDD	
6	Meter ID		
7	Meter Pressure		inch-Hg
8	Meter temp		°C
9	Ambient temp		°C
10	K-Factor		
11	VCC Coeff		
12	AL Coeff		
13	AX Coeff		
14	VE Coeff		
15	AX2 Coeff		
16	Serial Filter Length		Seconds
17	QC Filter Length		Seconds

**Engineering (eng1)**

08+330:23:59:50.899 12.25684 23.89813 0.4029922 0.2541656 233.4218 -  
 751.9 -8145.28 -1.386184 23.37653 23.37653 NAN

Field	Data	Units
1	RVDAS time tag	
2	Power Supply Voltage	V
3	Internal Case Temperature	°C
4	Pump #1 flow rate	L/min
5	Pump #2 flow rate	L/min
6	Pump #3 flow rate	L/min
7	Seismic air pressure	Lbs/sq-in
8	PIR case resistance (not currently hooked up, data is irrelevant)	Kohm
9	PIR case ratiometric output (not currently hooked up, data is irrelevant)	mV
10	Freezer #1 temperature	°C
11	Freezer #2 temperature	°C
12	Freezer #3 temperature	°C

\*See page 25 for PIR calculations.

On NBP1001 Field 12 was Altimiter (m) and Field 13 was Transmissometer (%). These values are relative values from the Yoyo Camera.

**Hydro-DAS (hdas)**

08+330:23:59:41.877 12.15836 14.22853 368.9655 4060.69 -1 65.5 65.5 80  
57

Field	Data	Units
1	RVDAS time tag	
2	Supply voltage	V
3	Panel temperature	°C
4	Fluorometer	mV
5	Transmissometer	mV
6	Sea Water Valve (-1 = stern thruster valve, 0 = moon pool valve)	
7	Flow meter 1 frequency	Hz
8	Flow meter 2 frequency	Hz
9	Flow meter 3 frequency	Hz
10	Flow meter 4 frequency	Hz

**GUV Data (pguv)**

08+330:23:59:40.328 112508 235940 .000197 1.856E-1 1.116E0 4.987E-2 -  
1.959E-4 1.637E0 4.153E-3 1.76E0 42.296 17.844

Field	Data	Units
1	RVDAS time tag	
2	Date	mmddyy
3	Time (UTC)	hhmmss
4	Ed0Gnd	V
5	Ed0320	uW (cm^2 nm)
6	Ed0340	uW (cm^2 nm)
7	Ed0313	uW (cm^2 nm)
8	Ed0305	uW (cm^2 nm)
9	Ed0380	uW (cm^2 nm)
10	Ed0PAR	uE (cm^2 nm)
11	Ed0395	uW (cm^2 nm)
12	Ed0Temp	°C
13	Ed0Vin	V

**Remote Temperature (rtmp)**

07+272:00:00:15.960 -1.7870

Field	Data	Units
1	RVDAS time tag	
2	Temperature at seawater intake	°C

## Navigational Data

### Seapath GPS (seap)

The Seapath GPS outputs the following data strings, four in NMEA format and two in proprietary PSXN format:

- GPZDA
- GPGGA
- GPVTG
- GPHDT
- PSXN, 20
- PSXN, 22
- PSXN, 23

#### GPZDA

02+253:00:00:00.772 \$GPZDA,235947.70,09,09,2002,,\*7F

Field	Data	Units
1	RVDAS time tag	
2	\$GPZDA	
3	time	hhmmss.ss
4	Day	dd
5	Month	mm
6	Year	yyyy
7	(empty field)	
8	Checksum	

#### GPGGA

02+253:00:00:00.938

GPGGA,235947.70,6629.239059,S,06827.668899,W,1,07,1.0,11.81,M,,M,,\*6F

Field	Data	Units
1	RVDAS time tag	
2	\$GPGGA	
3	time	hhmmss.ss
4	Latitude	ddmm.mmmmmmm
5	N or S for north or south latitude	
6	Longitude	ddmm.mmmmmmm
7	E or W for east or west longitude	
8	GPS quality indicator, 0=invalid, 1=GPS SPS, 2=DGPS, 3=PPS, 4=RTK, 5=float RTK, 6=dead reckoning	
9	number of satellites in use (00-99)	
10	HDOP	x.x
9	height above ellipsoid in meters	m.mm
11	M	
12	(empty field)	
13	M	
14	age of DGPS corrections in seconds	s.s
15	DGPS reference station ID (0000-1023)	
16	Checksum	

**GPVTG**

02+253:00:00:00.940 \$INVTG,19.96,T,,M,4.9,N,,K,A\*39

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	\$GPVTG	
3	course over ground, degrees true	d.dd
4	T	
5	,	
6	M	
7	speed over ground in knots	k.k
8	N	
9	,	
10	K	
11	Mode	
12	Checksum	

**GPHDT**

02+253:00:00:00.941 \$GPHDT,20.62,T\*23

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	\$GPHDT	
3	Heading, degrees true	d.dd
4	T	
5	Checksum	

**PSXN,20**

02+253:00:00:00.942 \$PSXN,20,0.43,0.43\*39

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	\$PSXN	
3	20	
4	Horizontal position & velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
5	Height & vertical velocity quality: 0=normal, 1=reduced performance, 2=invalid data	
6	Heading quality: 0=normal, 1=reduced performance, 2=invalid data	
7	Roll & pitch quality: 0=normal, 1=reduced performance, 2=invalid data	
8	Checksum	

**PSXN,22**

02+253:00:00:00.942 \$PSXN,22,0.43,0.43\*39

<b>Field</b>	<b>Data</b>	<b>Units</b>
1	RVDAS time tag	
2	\$PSXN	
3	22	
4	gyro calibration value since system start-up in degrees	d.dd
5	short term gyro offset in degrees	d.dd
6	Checksum	

**PSXN,23**

02+253:00:00:02.933 \$PSXN,23,0.47,0.57,20.62,0.03\*0C

Field	Data	Units
1	RVDAS time tag	
2	\$PSXN	
3	23	
4	roll in degrees, positive with port side up	d.dd
5	pitch in degrees, positive with bow up	d.dd
6	Heading, degrees true	d.dd
7	heave in meters, positive down	m.mm
8	Checksum	

**Trimble (P-Code) GPS (PCOD)**

The Trimble GPS, which formerly output Precise Position (*P*-Code) strings, but now only outputs Standard Position (*Civilian*) strings, outputs three NMEA standard data strings:

- Position fix (GGA)
- Latitude / longitude (GLL),
- Track and ground speed (VTG)

**GGA: GPS Position Fix – Geoid/Ellipsoid**01+319:00:04:11.193 \$GPGGA,000410.312,6227.8068,S,06043.6738,W,1,06,1.0,  
031.9,M,-017.4,M,,\*49

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGGA	
3	UTC time at position	hhmmss.sss
4	Latitude	ddmm.mmm
5	North (N) or South (S)	
6	Longitude	ddmm.mmm
7	East (E) or West (W)	
8	GPS quality: 0 = Fix not available or invalid 1 = GPS, SPS mode, fix valid 2 = DGPS (differential GPS), SPS mode, fix valid 3 = P-CODE PPS mode, fix valid	
9	Number of GPS satellites used	
10	HDOP (horizontal dilution of precision)	
11	Antenna height	meters
12	M for meters	
13	Geoidal height	meters
14	M for meters	
15	Age of differential GPS data (no data in the sample string)	
16	Differential reference station ID (no data in the sample string)	
17	Checksum (no delimiter before this field)	

**GLL: GPS Latitude/Longitude**

01+319:00:04:11.272 \$GPGLL,6227.8068,S,06043.6738,W,000410.312,A\*32

Field	Data	Units
1	RVDAS Time tag	
2	\$GPGLL	
3	Latitude	degrees
4	North or South	
5	Longitude	degrees
6	East or West	
7	UTC of position	hhmmss.sss
8	Status of data (A = valid)	
9	Checksum	

**VTG: GPS Track and Ground Speed**

01+319:00:04:11.273 \$GPVTG,138.8,T,126.0,M,000.0,N,000.0,K\*49

Field	Data	Units
1	RVDAS time tag	
2	\$GPVTG	
3	Heading	degrees
4	Degrees true (T)	
5	Heading	degrees
6	Degrees magnetic (M)	
7	Ship speed	knots
8	N = knots	
9	Speed	km/hr
10	K = km per hour	
11	Checksum	

**Gyro Compass (gyr1)**

00+019:23:59:59.952 \$HEHDT 25034,-020\*73

Field	Data	Units
1	RVDAS time tag	
2	\$HEHDT	
3	Heading, Degrees True	degrees
5	Checksum	

**ADCP Course (adcp)**

00+019:23:59:59.099 \$PUHAW,UVH,-1.48,-0.51,250.6

Field	Data	Units
1	RVDAS time tag	
2	\$PUHAW	
3	UVH (E-W, N-S, Heading)	
4	Ship Speed relative to reference layer, east vector	knots
5	Ship Speed relative to reference layer, north vector	knots
6	Ship heading	degrees

## **Processed Data**

The processed data sets can be found in the /process directory and subdirectories. Note: many of the subdirectories contain intermediate datasets to facilitate further processing and are not intended to be end-products. Only the final product files and datasets are described below.

### **pCO<sub>2</sub>-merged**

```
00+346:23:58:20.672 2000346.9991 2398.4 1008.4 0.01 45.4 350.3 342.6 15.77
Equil -43.6826 173.1997 15.51 33.90 0.33 5.28 9.05 1007.57 40.0 14.87 182.44 -1
```

Field	Data	Units
1	RVDAS time tag	
2	pCO <sub>2</sub> time tag (decimal is fractional time of day)	yyyyddd.ttt
3	Raw voltage (IR)	mV
4	Cell temperature	°C
5	Barometer	MBar
6	Concentration	ppm
7	Equilibrated temperature	°C
8	pCO <sub>2</sub> pressure	microAtm
9	Flow rate	ml / min
10	Source ID #	1 or 2 digits
11	Valve position	1 or 2 digits
12	Flow source (Equil = pCO <sub>2</sub> measurement)	text
13	RVDAS latitude	degrees
14	RVDAS longitude	degrees
15	TSG external temperature	°C
16	TSG salinity	PSU
17	TSG fluorometry	V
18	RVDAS true wind speed	m/s
19	RVDAS true wind direction	degrees
20	Barometric Pressure	mBars
21	Uncontaminated seawater pump flow rate	l/min
22	Speed over ground	knots
23	Course made good	degrees
24	Input Source	-1 stem Thurston; 0 moonpool

## Calculations

The file `instrument.coeff` located in the / directory contains the calibration factors for shipboard instruments. This was the file used by the RVDAS processing software.

### PAR

Coefficients `parc1` and `parcv` for this cruise can be found in the `instrument.coeff` file as the variable labeled PAR, respectively. Variable `par` is the raw data in mV, as described in the "mwx1" file description. The calibration scale and probe offset dark are values taken from the PAR Cal Sheet.

```
par = raw data mV
calibration scale = 5.8644 V/(μEinstiens/cm2sec)
parc1 = 1 / scale = .17
probe offset dark = -.1 mV
parcv = dark x 1000 mV/V = -0.0001 V
((par / 1000 mV/V) - parcv) x parc1 x 10000 cm2/m2 = μEinstiens/m2sec
```

Calculations (extracted from the C code):

```
/* Convert from mV to V */
par /= 1000;
/* (par V - vdark V) / Calibration Scale Factor V/uE/cm2sec */
parCalc = (par - parcv) * parc1 * 10000;
```

### PSP

Coefficient `pspCoeff` for this cruise can be found in the `instrument.coeff` file as the variable labeled PSP1. Variable `psp` is the raw data in mV, as described in the "mwx1" file description.

```
psp = raw data mV
calibration scale = pspCoeff x 10^-6 V/(W/m2)
psp / (scale x 1000 mV/V) = W/m2
```

Calculations (extracted from the C code):

```
/* Convert from mV to W/m^2 */
pspCalc = (psp * 1000 / pspCoeff);
```

## PIR

Coefficient pirCoeff for this cruise can be found in the instrument.coeff file as the variable labeled PIR1. Variable pir\_thermo is the raw data in mV, pir\_case is the PIR case temperature in Kelvins and pir\_dome is the PIR dome temperature in Kelvins, as described in the "mwx1" file description. Hard-coded "C" coefficients are shown below:

Dome constant = 3.5

Sigma = 5.6704e-8

```
pir_thermo = raw data mV
calibration scale = pirCoeff x 10^-6 V/(W/m^2)
pir_thermo / (scale x 1000 mV/V) = W/m^2
```

Calculations (extracted from the C code):

```
/* convert mV to W/m^2 */
pirCalc = (pir_thermo * 1000 / pirCoeff)
/* correct for case temperature */
pirCalc += sigma * pow(pir_case, 4)
/* correct for dome temperature */
pirCalc -= 3.5 * sigma * (pow(pir_dome, 4) - pow(pir_case, 4))
```

## Acquisition Problems and Events

This section lists problems with acquisition noted during this cruise including instrument failures, data acquisition system failures and any other factor affecting this data set. The format is ddd:hh:mm (ddd is year-day, hh is hour, and mm is minute). Times are reported in GMT.

Start	End	Description
007:00:00		Left Argentinean EEZ started loggers
057:23:59		Stopped logging LARISSA data.
058:08:40		Entered Argentinean EEZ
060:		68° West – stopped loggers

We currently have a known error in the Trimble (P-Code) GPS (PCOD) data. It is not collecting the right date. It is a firmware problem. The time is accurate (for a GPS) but the date constantly says 15-07-90.

## Appendix: Sensors and Calibrations

### NBP1001 Shipboard Sensors

Sensor	Serial Number	Last Calibration Date	Comments
<b>Meteorology &amp; Radiometers</b>			
Port Anemometer (Gill Ultrasonic)	836076	5/15/2007	Installed 12/13/2008 There are no cal-sheets for this instrument.
Stbd Anemometer (Gill Ultrasonic)	071739	5/15/2007	Installed 11/15/2009 There are no cal-sheets for this instrument.
Barometer	01705	03/05/2009	Installed 12/19/09
Humidity/Wet Temp	6135	7/30/2008	Installed 10/7/2009
PIR	32845F3	10/14/2008	Installed 10/15/2009
PSP	32850F3	10/14/2008	Installed 10/15/2009
Mast PAR	6357	2/7/2008	Installed 10/15/09
GUV (Mast)	25110203114	7/16/08	Installed 2/28/09
<b>Underway</b>			
Micro TSG	4550449-0242	3/31/2008	Installed 4/1/2009
Remote Temp (primary)	3846730-0323	2/06/2008	Installed 10/07/2009
Remote Temp (secondary)	031267	4/12/2006	Installed 1/29/2007
Fluorometer	AFLD-011	10/29/2008	Installed 1/01/2009
Transmissometer	CST-831	4/9/2008	Installed 11/18/09

**NBP1001 CTD Sensors**

Sensor	Serial Number	Last Calibration Date	Comments
CTD Deck Unit	11P19858-0768	N/A	
Slip-Ring Assembly	1.406	N/A	
Carousel Water Sampler	3211265-0066	N/A	
CTD Fish	09P10716-0377	11/4/2008	
CTD Fish Pressure	58949	11/4/2008	
Conductivity (primary)	041143	2/5/2009	
Conductivity (secondary)	041798	2/5/2009	
Temperature (primary)	031541	9/23/2008	
Temperature (secondary)	03P2186	9/24/2008	
Pump (primary)	051626	4/17/2008	
Pump (secondary)	051627	4/27/2008	
Dissolved O2 (primary)	0139	4/21/2009	
Dissolved O2 (secondary)	0155	4/21/2009	
Fluorometer	AFL-016D	2/24/2009	
Transmissometer	CST-892DR	4/9/2008	
PAR	4361	10/16/2008	
Altimeter	47042	N/A	
SPAR	6357	2/7/2008	See mast PAR for details
Bottom Contact Switch	2	N/A	

**Calibrations**

The following pages are replicas of current calibration sheets for the sensors used during this cruise.

## Gravity Tie Start (Punta Arenas)

**Gravity Tie Spreadsheet**

**The fields outlined in BOLD MUST BE FILLED IN for this spreadsheet to operate properly.**  
**The automatically calculated values show up in the shaded fields.**

Date:	12/21/2009	Reference Code Numbers:
Location:	Punta Arenas, Chile	Station no. 9337-50
Station:	Harbour Admin. Bldg.	ISGN no. 51230N
Latitude:	53 09 S	
Longitude:	070 55 W	
Elevation:		
Gravity:	981320.82	

Value	Time (GMT)
Ship's meter before gravity tie ( Gravity (cu) )	8979.2
Ship's meter after gravity tie ( Gravity (cu) )	8979.1
Average	8979.2
Ship Gravimeter's Calibration Constant	1.0046
Corrected ship's meter ( QC Grav (mgal) )	9020.5

Value	Time (GMT)
Ship's meter before gravity tie (serial, RVDAS)	8979.0
Ship's meter after gravity tie (serial, RVDAS)	8979.4
Average (for comparison check only)	8979.2

Portable Gravimeter Interval Factor	1.01007	From Table 1 of Model G #807 Meter
-------------------------------------	---------	------------------------------------

Station	Value	Time (GMT)	Temp	Date
Pier measurement 1	4914.47	12:40	54	December 21, 2009
Pier measurement 2	4914.53	12:43	54	December 21, 2009
Pier measurement 3	4914.46	12:45	54	December 21, 2009
Average	4914.49			
Station measurement 1	4915.18	13:00	54	December 21, 2009
Station measurement 2	4915.11	13:04	54	December 21, 2009
Station measurement 3	4915.13	13:08	54	December 21, 2009
Average	4915.14			
Pier measurement 4	4914.47	13:30	54	December 21, 2009
Pier measurement 5	4914.54	13:35	54	December 21, 2009
Pier measurement 6	4914.44	13:40	54	December 21, 2009
Average	4914.48			

Gravity offset from last tie	972299.85
Drift since last tie	0.00

OBS Differences	Comments
-0.66	
-0.66	
-0.66	
981320.16	Gravity tie performed by Sheldon Blackman and Tony D'Aoust. Conditions were pretty good considering there was a lot of dock activity. The was not too unstable.
0.5	
0.3	
981320.31	
972299.85	

Note about Elevation of Pier: If pier is below the ship's gravimeter, this value is negative. If above, positive.

**Barometer**

**R.M. Young Company**  
2801 Aero Park Drive  
Traverse City, Michigan 49686 USA

**CALIBRATION REPORT**  
**Barometric Pressure Sensor**

Customer: *Raytheon Technical Services Co LLC*

Test Number: 93052  
Test Date: 5 March 2009

Customer PO: RR44553-01  
Sales Order: 0282

Model: 61201	Serial Number: BP01705
Description: Barometric Pressure Sensor	

Report of calibration comparison of test barometric pressure sensor with National Institute of Standards and Technology traceable standard pressure calibrator at five pressures in the R.M. Young Company controlled pressure facility. Calibration accuracy  $\pm 1.0$  hPa.

Reference Pressure (hPa)	Voltage Output (millivolts)	Indicated (1) Pressure (hPa)
800.0	1	800.1
875.0	1251	875.1
950.0	2501	950.1
1025.0	3750	1025.0
1100.0	4998	1099.9

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument	Serial # NIST Test Reference
Druck Pressure Controller Model DPI515	51500497 UKAS Lab 0221
Fluke Multimeter Model 8060A	4865407 234027

Tested By: *EChamney*

M E T E O R O L O G I C A L   I N S T R U M E N T S

Tel: 231-946-3980 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com

**Humidity Sensor**

**R.M. Young Company**  
2801 Aero Park Drive  
Traverse City, Michigan 49686 USA

**CALIBRATION REPORT****Relative Humidity Sensor**

Customer: *Raytheon Technical Services Co LLC*

Test Number: 87910R  
Test Date: 31 July 2008

Customer PO: RR41221-01  
Sales Order: 9867

Test Sensor:	Serial Number: 6135
Model: 41372LC	Description: Temperature/Relative Humidity Sensor

Report of calibration comparison of test relative humidity sensor with National Institute of Standards and Technology traceable standard relative humidity sensor at five humidity levels in the R.M. Young Company controlled humidity chamber facility. Calibration accuracy  $\pm 2.0\%$ .

Reference Humidity (%)	Current Output (milliamps)	Indicated (1) Humidity (%)
10.0	5.9	11.6
30.0	8.8	30.0
50.0	12.1	50.7
70	15.1	69.6
90	18.0	87.2

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

<u>Reference Instrument</u>	<u>Serial #</u>	<u>NIST Test Reference</u>
Vaisala Humidity Sensor Model 35AC	N475040	TN 266152
Fluke Multimeter Model 8060A	4865407	234027

Tested By: E. Chenuary

M E T E O R O L O G I C A L   I N S T R U M E N T S

tel: 231-946-3990 fax: 231-946-4772 email: met.sales@youngusa.com website: www.youngusa.com

***Wet Temperature (part of humidity) Sensor***

R.M. Young Company  
2801 Aero Park Drive  
Traverse City, Michigan 49686 USA

**CALIBRATION REPORT**  
**Temperature Sensor**

Customer: Raytheon Technical Services Co LLC

Test Number: 87910  
Test Date: 30 July 2008

Customer PO: RR41221-01  
Sales Order: 9867

Test Sensor:	
Model: 41372LC	Serial Number: 6135
Description: Temperature/Relative Humidity Sensor	

Report of calibration comparison of test temperature sensor with National Institute of Standards and Technology traceable standard thermometers at three temperatures in the R.M. Young Company controlled temperature calibration bath facilities. Calibration accuracy  $\pm 0.1^\circ$  Celsius.

Bath Temperature (degrees C)	Current Output (milliamps)	Indicated (1) Temperature (degrees C)
-49.93	4.009	-49.94
0.03	12.006	0.04
49.92	19.986	49.91

(1) Calculated from current output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument	Serial #	NIST Test Reference
Brooklyn Thermometer Model 43-FC	8006-118	204365
Brooklyn Thermometer Model 22332-D5-FC	25071	249763
Brooklyn Thermometer Model 2X400-D7-FC	77532	228060
Keithley Multimeter Model 191	15232	234027

Tested By: E.Cheney

M E T E O R O L O G I C A L   I N S T R U M E N T S

Tel: 231-946-3990 Fax: 231-946-4772 Email: met.sales@youngusa.com Website: www.youngusa.com

**PIR****THE EPPLEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA  
 Telephone: 401-847-1020      Fax: 401-847-1031  
 Email: info@eppleylab.com

Internet: [www.eppleylab.com](http://www.eppleylab.com)

**STANDARDIZATION OF  
EPPLEY PRECISION INFRARED RADIOMETER  
Model PIR**

Serial Number: 32845P3

Resistance: 713 Ω at 23 °C  
 Temperature Compensation Range: -20 to +40 °C

This pyrgeometer has been compared against Eppley's Blackbody Calibration System; under radiation intensities of approximately 200 watts meter<sup>-2</sup> and an average ambient temperature of 24 °C as measured by Standard Omega Temperature Probe, RTD#1.

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$4.15 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 700 watts meter<sup>-2</sup>. This radiometer is linear to within ±1.0% up to this intensity.

The calibration of this instrument is traceable to the International Practical Temperature Scale (IPTS) through a precision low-temperature blackbody.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".

Shipped to National Science Foundation Date of Test: Sept. 30, 2008  
 Port Hueneme, CA

In Charge of Test: *B. Eppley*

S.O. Number: 61816  
 Date: October 14, 2008

Reviewed by: *[Signature]*

Remarks:

**PSP****THE EPPELEY LABORATORY, INC.**

12 Sheffield Ave., P.O. Box 419, Newport, RI 02840 USA

Telephone: 401-847-1020

Fax: 401-847-1031

Email: info@eppleylab.com

Internet: www.eppleylab.com



Scientific Instruments  
for Precision Measurements  
Since 1917

**STANDARDIZATION OF  
EPPELEY PRECISION SPECTRAL PYRANOMETER  
Model PSP**

Serial Number: 32850F3

Resistance: 706 Ω at 23 °C

Temperature Compensation Range: -20 to +40 °C

This radiometer has been compared with Standard Precision Spectral Pyranometer, Serial Number 21231F3 in Eppley's Integrating Hemisphere under radiation intensities of approximately 700 watts meter<sup>-2</sup> (roughly one half a solar constant).

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$7.89 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 1400 watts meter<sup>-2</sup>. This radiometer is linear to within ± 0.5% up to this intensity.

The calibration of this instrument is traceable to standard self-calibrating cavity pyrheliometers in terms of the Systems Internationale des Unites (SI units), which participated in the Tenth International Pyrheliometric Comparisons (IPC X) at Davos, Switzerland in September-October 2005.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".

Useful conversion facts: 1 cal cm<sup>-2</sup> min<sup>-1</sup> = 697.3 watts meter<sup>-2</sup>  
1 BTU/ft<sup>2</sup>·hr<sup>-1</sup> = 3.153 watts meter<sup>-2</sup>

Shipped to: National Science Foundation Date of Test: Sept. 24, 2008  
Port Hueneme, CA

S.O. Number: 61817  
Date: Oct. 14, 2008

In Charge of Test: *R. Eggeman*Reviewed by: *Thomas Kuh*

Remarks:

**Mast PAR****Biospherical Instruments Inc.****CALIBRATION CERTIFICATE**

Calibration Date 2/7/2008  
 Model Number QSR-240  
 Serial Number 6357  
 Operator TPO  
 Standard Lamp 91537(10/25/2008)  
 Probe Excitation Voltage Range: 6 to 18 VDC(+)  
 Output Polarity: Positive

Probe Conditions at Calibration(in air):

Calibration Voltage: 6 VDC(+)  
 Probe Current: 7.2 mA

Probe Output Voltage:

Probe Illuminated	<u>84.5</u>	mV
Probe Dark	<u>2.0</u>	mV
Probe Net Response	<u>82.5</u>	mV
RG780	<u>4.2</u>	mV

Corrected Lamp Output:Output in Air (same condition as calibration):

8.83E+15 quanta/cm<sup>2</sup>sec  
0.01467  $\mu\text{E}/\text{cm}^2\text{sec}$

Calibration Scale Factor:

(To calculate Irradiance, divide the net voltage reading in Volts by this value.)

Dry: 9.3380E-18 V/(quanta/cm<sup>2</sup>sec)  
5.6234E+00 V/( $\mu\text{E}/\text{cm}^2\text{sec}$ )

Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with isopropanol.
4. Calibration was performed with customer cable, when available.

**GUV (Mast)**

GUV-2511 Calibration Certificate											
System Serial Number 25110203114 Calibration database 25110203114v5.mdb DASSN 0069 Microprocessor Tag Number 4				Date of Calibration 7/16/08 Date of Certificate 7/16/2008 Standard of Spectral Irradiance 91537(10/25/06) Operator TC							
Monochromatic Channels	Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	ScaleSmall [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	ScaleMedium [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	ScaleLarge [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$ ]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units	
Ed0320	2	320	2.4512E-10	2.5002E-05	7.3046E-03	2.3055E+00	6.1000E-05	6.5000E-05	5.7800E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$	
Ed0340	6	340	1.9263E-10	1.9648E-05	5.7404E-03	1.9692E+00	1.0800E-04	1.1200E-04	8.6600E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$	
Ed0313	8	313	2.3098E-10	2.3560E-05	6.8833E-03	2.4163E+00	8.8200E-04	8.7800E-04	-1.5570E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$	
Ed0306	10	305	1.2230E-11	1.2474E-06	3.6444E-04	1.2526E-01	4.2000E-04	4.2300E-04	1.1910E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$	
Ed0380	12	380	8.3732E-11	8.5406E-06	2.4952E-03	8.0032E-01	2.7300E-04	2.7100E-04	-1.2200E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$	
Ed0396	16	395	2.9823E-10	3.0419E-05	8.8871E-03	2.8092E+00	3.9200E-04	3.9500E-04	1.4740E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$	
Broadband Channels	Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	ScaleSmall [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	ScaleMedium [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	ScaleLarge [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$ ]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units	
Ed0PAR	13	400-700	1.7494E-05	1.7844E+00	5.2131E+02	1.8424E+05	5.7900E-04	5.8200E-04	1.3130E-03	$\mu\text{E}/(\text{cm}^2\cdot\text{sec})$	
Auxiliary Channels	Address	Wavelength	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement Units	
Ed0Temp	22	0	1.0000E+00	1.0000E-02	1.0000E-02	1.0000E-02	0.0000E+00	0.0000E+00	0.0000E+00	C	
Ed0Vin	27	0	1.0000E+00	-2.5000E-01	-2.5000E-01	-2.5000E-01	0.0000E+00	0.0000E+00	0.0000E+00	V	

© Biospherical Instruments Inc., 5340 Riley Street, San Diego, California 92110 USA. Contact [support@biospherical.com](mailto:support@biospherical.com) for more information.

Calibration Data – Do Not Destroy

page 2 of 2

***Micro-TSG (Temperature)***

63

**SEA-BIRD ELECTRONICS, INC.**  
**1808 136th Place N.E., Bellevue, Washington, 98005 USA**  
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0242  
 CALIBRATION DATE: 31-Mar-08

SBE45 TEMPERATURE CALIBRATION DATA  
 ITS-90 TEMPERATURE SCALE

## ITS-90 COEFFICIENTS


a0 = -3.912618e-006  
 a1 = 2.847375e-004  
 a2 = -3.193105e-006  
 a3 = 1.720429e-007

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	649832.1	1.0000	0.0000
4.5000	554895.8	4.5000	-0.0000
15.0000	352330.7	15.0000	0.0000
18.5000	304721.7	18.5000	-0.0000
24.0000	244015.9	24.0000	0.0000
29.0000	200610.7	29.0000	-0.0000
32.5000	175490.5	32.5000	0.0000

$$\text{Temperature ITS-90} = 1/[a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]] - 273.15 \text{ (}^\circ\text{C)}$$

Residual = instrument temperature - bath temperature

Date, Delta T (mdeg C)

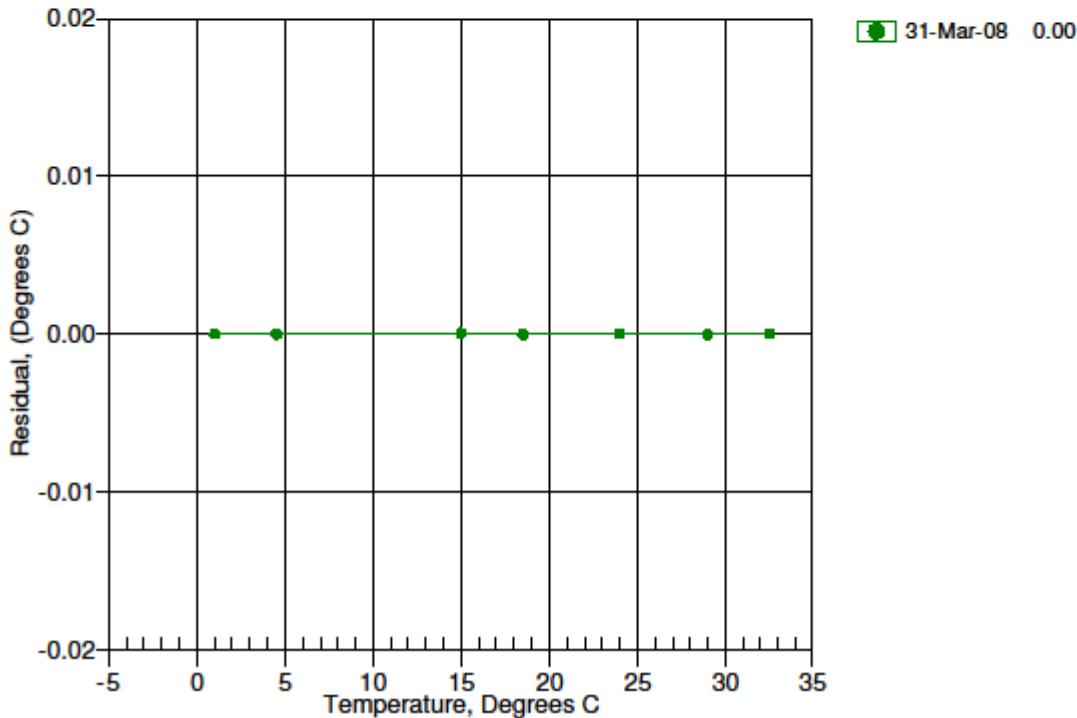

***Micro-TSG (Conductivity)***

64

**SEA-BIRD ELECTRONICS, INC.**  
**1808 136th Place N.E., Bellevue, Washington, 98005 USA**  
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0242  
 CALIBRATION DATE: 31-Mar-08

SBE 45 CONDUCTIVITY CALIBRATION DATA  
 PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

**COEFFICIENTS:**

$g = -9.980367e-001$	$CPcor = -9.5700e-008$
$h = 1.523293e-001$	$CTcor = 3.2500e-006$
$i = -4.438334e-004$	$WBOTC = 0.0000e+000$
$j = 5.882995e-005$	

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (Hz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2565.99	0.00000	0.00000
1.0000	34.8739	2.98042	5122.83	2.98043	0.00002
4.5000	34.8542	3.28795	5316.56	3.28793	-0.00001
15.0000	34.8112	4.27105	5892.53	4.27104	-0.00001
18.5000	34.8020	4.61668	6081.77	4.61667	-0.00001
24.0000	34.7913	5.17532	6375.44	5.17535	0.00003
29.0000	34.7843	5.69767	6637.87	5.69765	-0.00002


$$f = \text{INST FREQ} * \sqrt{1.0 + WBOTC * t} / 1000.0$$

$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / (1 + \delta t + \epsilon p) \text{ Siemens/meter}$$

t = temperature [°C]; p = pressure[decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;

Residual = instrument conductivity - bath conductivity

Date, Slope Correction

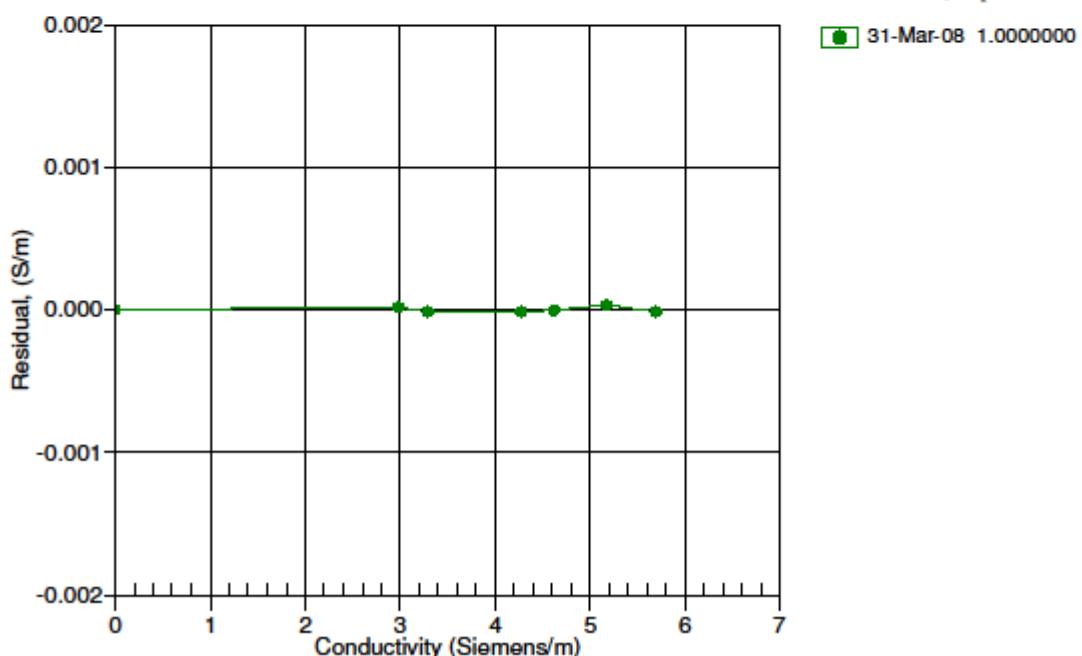

## Remote Temperature (Primary)

**SEA-BIRD ELECTRONICS, INC.**  
**1808 136th Place N.E., Bellevue, Washington, 98005 USA**  
**Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com**

SENSOR SERIAL NUMBER: 0323  
 CALIBRATION DATE: 06-Feb-08

SBE 38 TEMPERATURE CALIBRATION DATA  
 ITS-90 TEMPERATURE SCALE

**ITS-90 COEFFICIENTS**


a<sub>0</sub> = 1.043750e-005  
 a<sub>1</sub> = 2.759391e-004  
 a<sub>2</sub> = -2.392123e-006  
 a<sub>3</sub> = 1.581561e-007


BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.50010	711112.1	-1.50006	0.00004
0.99990	635155.2	0.99989	-0.00001
4.50000	543802.3	4.49989	-0.00011
7.99990	467105.6	7.99993	0.00003
11.50000	402495.3	11.50004	0.00004
15.00000	347890.5	15.00002	0.00002
18.49990	301592.6	18.49996	0.00006
22.00000	262214.9	21.99994	-0.00006
25.49990	228622.2	25.49990	-0.00000
29.00000	199879.6	28.99991	-0.00009
32.50000	175215.8	32.50007	0.00007

$$\text{Temperature ITS-90} = 1/\{a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]\} - 273.15 \text{ (°C)}$$

Residual = instrument temperature - bath temperature

Date, Delta T (mdeg C)

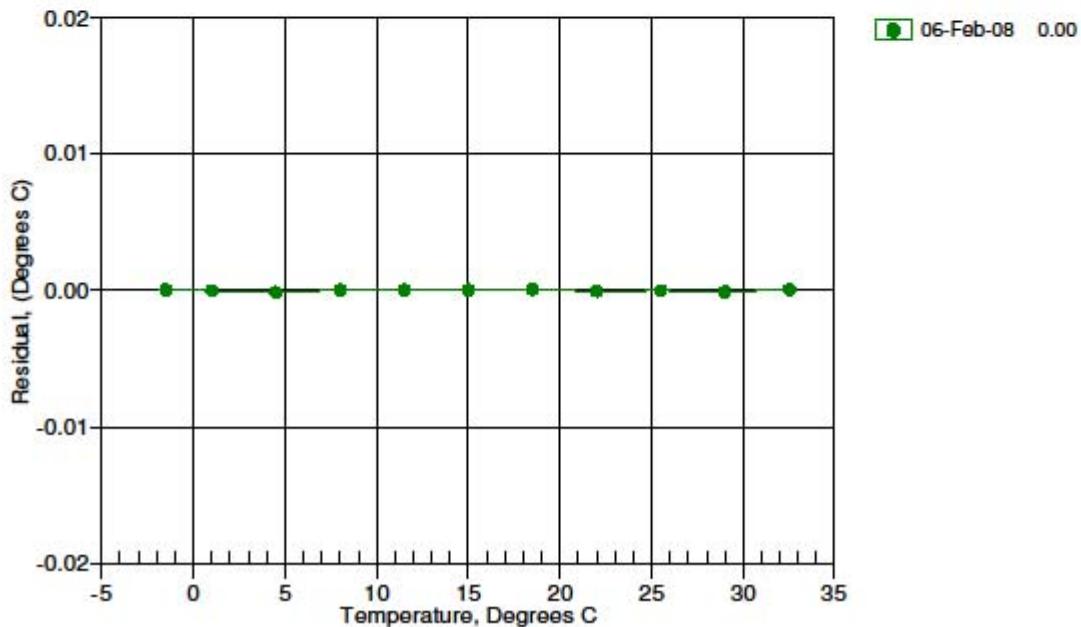

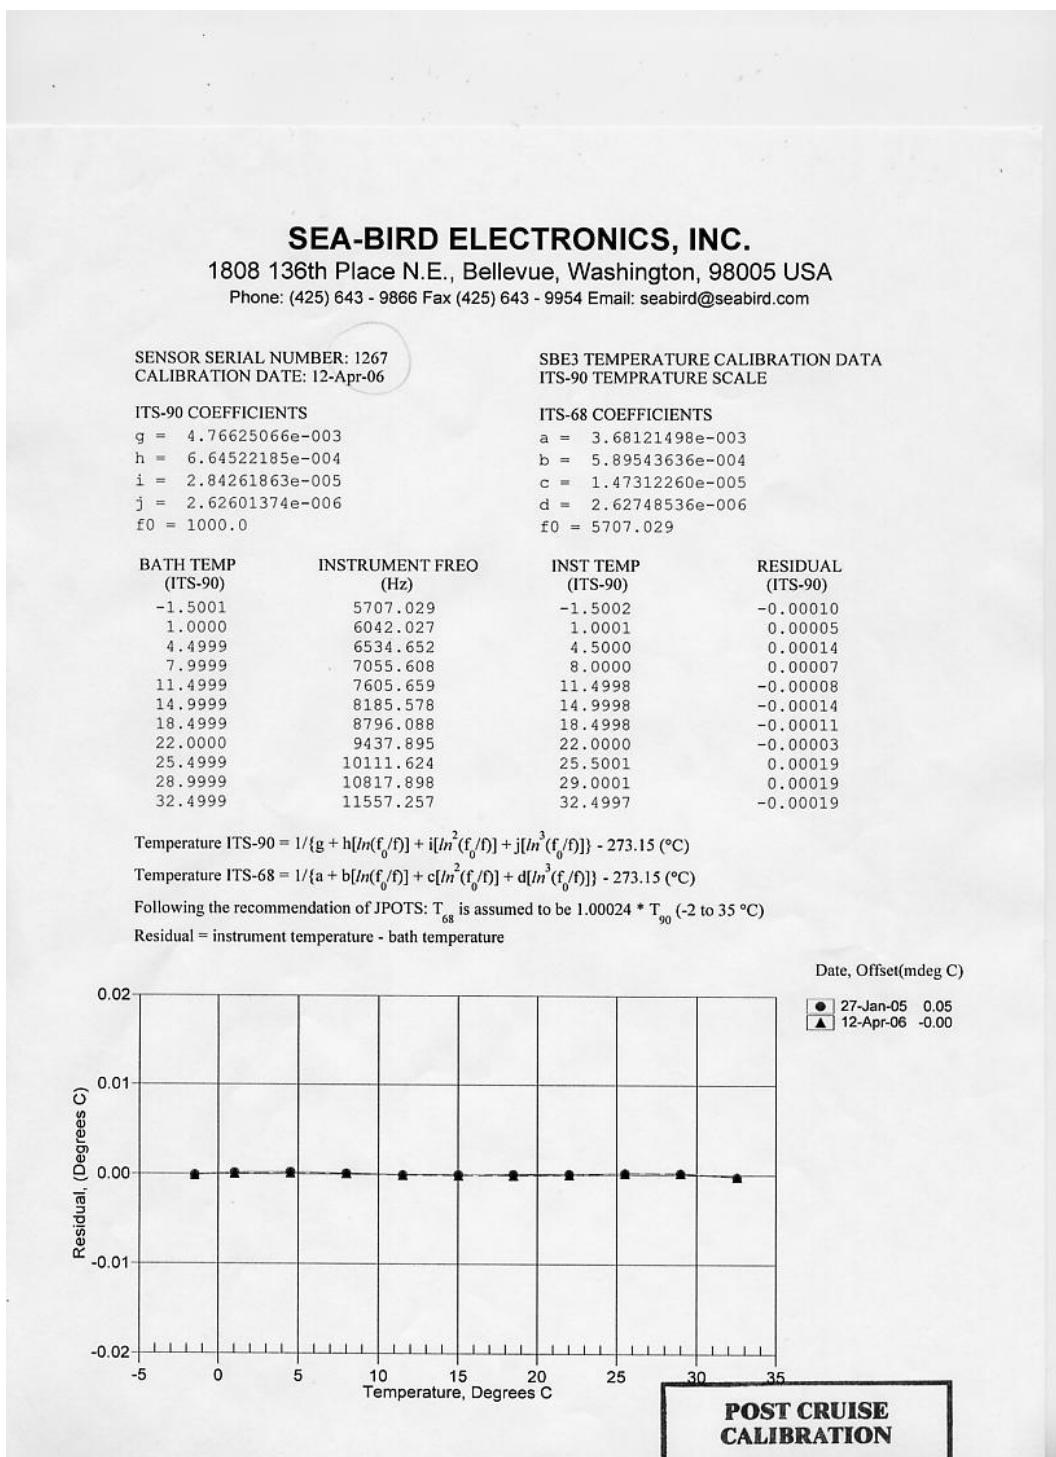**Remote Temperature (Secondary)**

***Underway fluorometer***

PO Box 518  
620 Aplegate St.  
Philomath OR 97370



(541) 929-5650  
Fax (541) 929-5277  
<http://www.wetlabs.com>

**Chlorophyll Fluorometer Characterization .**

Date: 10/29/08  
Serial #: AFLD-011  
Job#: 0011007  
Tech: K.C

Dark Counts 0.183 volts  
CEV 2.902 volts  
SF 8.6598

FSV 5.36 volts

Linearity: 0.999 R<sup>2</sup> (0–1.5 volts)  
0.995 R<sup>2</sup> (0– 5.45 volts)

**Notes:**

**Dark Counts:** Signal output of the meter in clean water with black tape over detector.

**CEV** is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to 25 µg/l of a *Thalassiosira weissflogii* phytoplankton culture.

**SF** is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determine by using the following equation:  
SF = (25) / (CEV – dark) e.g.(25 / (2.865 – 0.238) = 9.516)

**FSV** is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m<sup>3</sup>) can be derived by using the following equation: (µg/l) = (Vmeasured - dark) \* SF

The relationship between fluorescence and chlorophyll-a concentrations in-situ is high variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [ Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

***Underway Transmissometer***

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 929-5650  
Fax (541) 929-5277  
[www.wetlabs.com](http://www.wetlabs.com)

**C-Star Calibration**

Date	April 9, 2008	S/N#	CST-831	Pathlength	25 cm
------	---------------	------	---------	------------	-------

Analog meter	
V <sub>d</sub>	0.061 V
V <sub>air</sub>	4.838 V
V <sub>ref</sub>	4.767 V

Temperature of calibration water	22.9 °C
Ambient temperature during calibration	26.0 °C

Relationship of transmittance (Tr) to beam attenuation coefficient (c), and pathlength (x):  $Tr = e^{-cx}$

To determine beam transmittance:  $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient:  $c = -1/x * \ln(Tr)$

**V<sub>d</sub>** Meter output with the beam blocked. This is the offset.  
**V<sub>air</sub>** Meter output in air with a clear beam path.  
**V<sub>ref</sub>** Meter output with clean water in the path.  
 Temperature of calibration water: temperature of clean water used to obtain V<sub>ref</sub>.  
 Ambient temperature: meter temperature in air during the calibration  
**V<sub>sig</sub>** Measured signal output of meter.

## CTD Fish & Pressure Sensor

### SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0377  
CALIBRATION DATE: 04-Nov-08

SBE9plus PRESSURE CALIBRATION DATA  
10000 psia S/N 58949

DIGIQUARTZ COEFFICIENTS:

C1 = -4.840395e+004  
C2 = -2.017057e-003  
C3 = 1.464810e-002  
D1 = 3.990600e-002  
D2 = 0.000000e+000  
T1 = 2.998386e+001  
T2 = -2.560542e-004  
T3 = 3.869120e-006  
T4 = 2.452640e-009  
T5 = 0.000000e+000


AD590M, AD590B, SLOPE AND OFFSET:

AD590M = 1.14600e-002  
AD590B = -8.45734e+000  
Slope = 0.99993  
Offset = 0.3479 (dbars)

PRESSURE (PSIA)	INST OUTPUT(Hz)	INST TEMP(C)	INST OUTPUT (PSIA)	CORRECTED INST OUTPUT (PSIA)	RESIDUAL (PSIA)
14.481	33360.00	19.3	14.073	14.577	0.096
2001.608	34036.60	19.4	2001.032	2001.389	-0.219
3988.829	34698.10	19.4	3988.692	3988.901	0.072
5975.782	35345.00	19.5	5975.900	5975.961	0.179
7961.793	35977.90	19.5	7961.992	7961.906	0.113
9949.713	36598.40	19.5	9949.725	9949.491	-0.222
7962.802	35978.20	19.5	7962.922	7962.835	0.033
5975.849	35345.00	19.7	5975.808	5975.869	0.020
3988.776	34698.10	19.7	3988.589	3988.798	0.022
2001.616	34036.70	19.7	2001.214	2001.571	-0.045
14.489	33360.00	19.7	13.933	14.438	-0.051

Residual = corrected instrument pressure - reference pressure

Date, Avg Offset(psia)

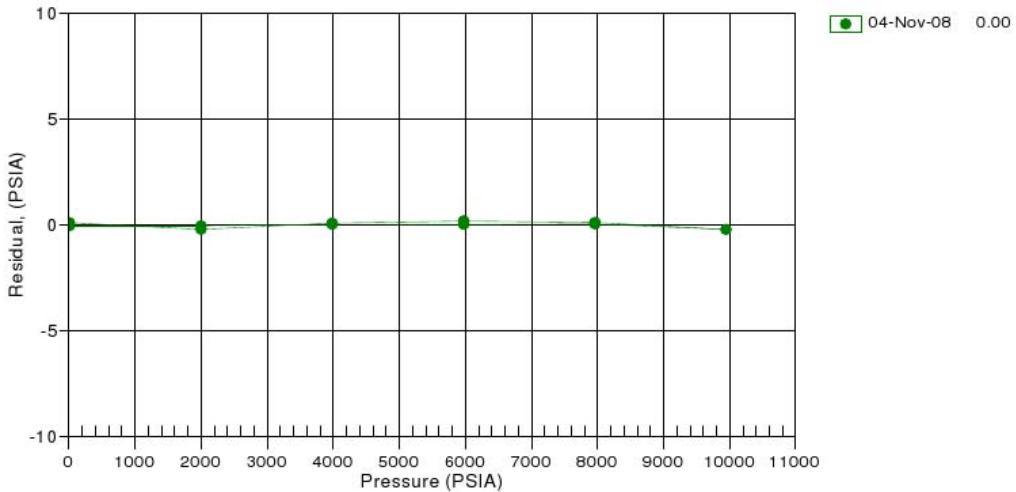

## CTD Conductivity (Primary)

**SEA-BIRD ELECTRONICS, INC.**  
 1808 136th Place N.E., Bellevue, Washington, 98005 USA  
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1143  
 CALIBRATION DATE: 05-Feb-09

SBE4 CONDUCTIVITY CALIBRATION DATA  
 PSS 1978: C(35,15,0) = 4.2914 Scimens/meter

GHIJ COEFFICIENTS

g = -3.93837922e+000  
 h = 5.02919775e-001  
 i = 1.74294974e-005  
 j = 2.57281394e-005  
 CPcor = -9.5700e-008 (nominal)  
 CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 3.45879761e-005  
 b = 5.02904266e-001  
 c = -3.93813469e+000  
 d = -8.04200177e-005  
 m = 3.9  
 CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.79770	0.00000	0.00000
-1.0000	34.8651	2.80814	7.96520	2.80816	0.00002
1.0000	34.8653	2.97975	8.17513	2.97975	-0.00000
14.9999	34.8661	4.27706	9.61308	4.27702	-0.00005
18.4999	34.8656	4.62419	9.96221	4.62421	0.00001
29.0000	34.8638	5.70922	10.98066	5.70928	0.00006
32.5000	34.8588	6.08256	11.30933	6.08252	-0.00004


$$\text{Conductivity} = (g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p) \text{ Siemens/meter}$$

$$\text{Conductivity} = (af^m + bf^2 + c + dt) / [10 (1 + \epsilon p)] \text{ Siemens/meter}$$

t = temperature[°C]; p = pressure[decibars];  $\delta$  = CTcor;  $\epsilon$  = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

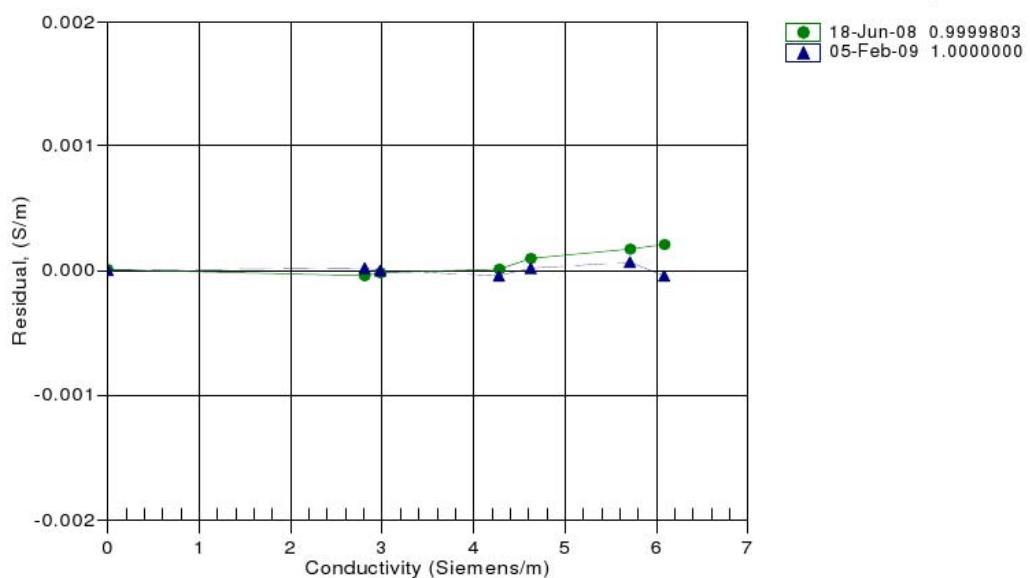

## ***CTD Conductivity (Secondary)***



### **Conductivity Calibration Report**

Customer:	Raytheon Polar Services Co.		
Job Number:	53449	Date of Report:	2/5/2009
Model Number:	SBE 04C	Serial Number:	041798

*Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.*

*An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.*

'AS RECEIVED CALIBRATION'	<input checked="" type="checkbox"/> Performed	<input type="checkbox"/> Not Performed
Date: <input type="text" value="2/5/2009"/>	Drift since last cal: <input type="text" value="+0.00030"/>	PSU/month*
Comments:		

'CALIBRATION AFTER CLEANING & REPLATINIZING'	<input type="checkbox"/> Performed	<input checked="" type="checkbox"/> Not Performed
Date: <input type="text"/>	Drift since Last cal: <input type="text"/>	PSU/month*
Comments:		

*\*Measured at 3.0 S/m*

*Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.*

## CTD Temperature (Primary)

**SEA-BIRD ELECTRONICS, INC.**  
**1808 136th Place N.E., Bellevue, Washington, 98005 USA**  
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1541  
 CALIBRATION DATE: 23-Sep-08

SBE3 TEMPERATURE CALIBRATION DATA  
 ITS-90 TEMPERATURE SCALE

ITS-90 COEFFICIENTS

g = 4.82572133e-003  
 h = 6.66033690e-004  
 i = 2.42074968e-005  
 j = 1.85024492e-006  
 f0 = 1000.0

IPTS-68 COEFFICIENTS

a = 3.68121447e-003  
 b = 5.96384959e-004  
 c = 1.41191264e-005  
 d = 1.85158060e-006  
 f0 = 6185.962


BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5002	6185.962	-1.5002	0.00004
0.9998	6544.716	0.9998	0.00001
4.4999	7071.817	4.4998	-0.00013
7.9998	7628.647	7.9998	-0.00004
11.4999	8216.031	11.5000	0.00007
14.9998	8834.694	15.0001	0.00030
18.4998	9485.283	18.4996	-0.00018
21.9999	10168.745	21.9997	-0.00017
25.4998	10885.667	25.4998	0.00003
28.9998	11636.718	28.9999	0.00010
32.4998	12422.500	32.4998	-0.00003

$$\text{Temperature ITS-90} = 1/(g + h[\ln(f/f_0)] + i[\ln^2(f/f_0)] + j[\ln^3(f/f_0)]) - 273.15 \text{ (\textdegree C)}$$

$$\text{Temperature IPTS-68} = 1/(a + b[\ln(f/f_0)] + c[\ln^2(f/f_0)] + d[\ln^3(f/f_0)]) - 273.15 \text{ (\textdegree C)}$$

Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 \times T_{90}$  (-2 to 35  $\text{\textdegree C}$ )

Residual = instrument temperature - bath temperature

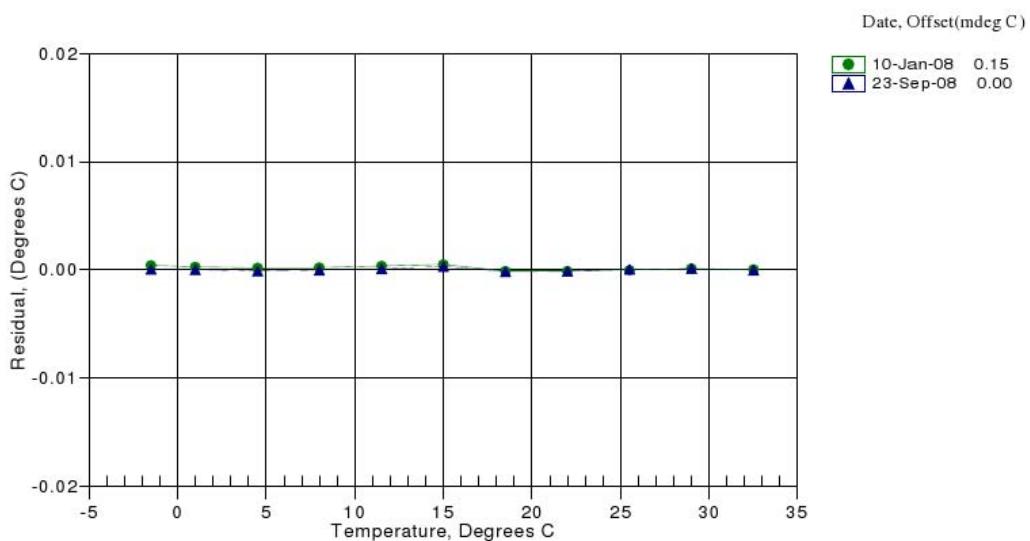

## CTD Temperature (Secondary)

### SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 2186  
CALIBRATION DATE: 24-Sep-08

SBE3 TEMPERATURE CALIBRATION DATA  
ITS-90 TEMPERATURE SCALE

#### ITS-90 COEFFICIENTS

g = 4.34024834e-003  
h = 6.44803145e-004  
i = 2.33555779e-005  
j = 2.21914616e-006  
f0 = 1000.0

#### IPTS-68 COEFFICIENTS

a = 3.68121489e-003  
b = 6.02962056e-004  
c = 1.63357947e-005  
d = 2.22071359e-006  
f0 = 2882.286

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.5002	2882.286	-1.5002	0.00001
0.9998	3047.601	0.9998	0.00001
4.4998	3290.416	4.4998	-0.00003
7.9998	3546.845	7.9998	-0.00003
11.4998	3817.254	11.4998	0.00003
14.9998	4101.993	14.9999	0.00008
18.4998	4401.393	18.4998	-0.00001
21.9998	4715.801	21.9997	-0.00007
25.4998	5045.545	25.4998	-0.00001
28.9998	5390.920	28.9998	0.00003
32.4998	5752.215	32.4998	-0.00000


$$\text{Temperature ITS-90} = 1/(g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]) - 273.15 (\text{°C})$$

$$\text{Temperature IPTS-68} = 1/(a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]) - 273.15 (\text{°C})$$

Following the recommendation of JPOTS:  $T_{68}$  is assumed to be  $1.00024 \times T_{90}$  (-2 to 35 °C)

Residual = instrument temperature - bath temperature

Date, Offset(mdeg C)

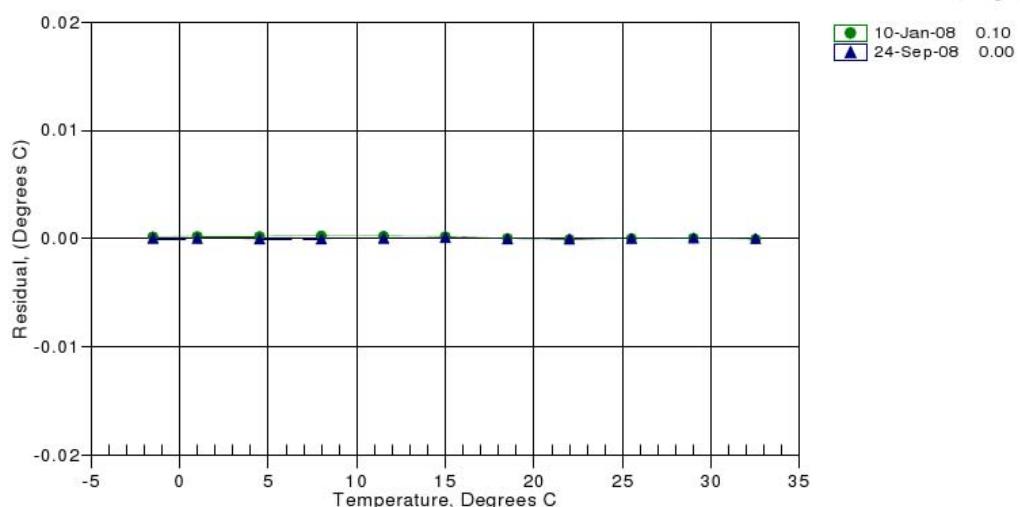

***CTD Pump (Primary)*****NBP-Bird Electronics, Inc**

53° 10'S, 70° 50'W, Punta Arenas, Chile

Phone: (808)434-9769, (808)659-5076 Fax: 011-870-336-661-014

Email: et@NBP.usap.gov

**SBE 5+ Pump Service & Calibration**

4/17/08

S/N 051626

X Check all O-rings, lubricate and install new O-rings if requiredX Check Thrust Washers, replace if necessaryX Remove and clean impeller – reinstallX Tune R11 as necessary for RPM adjustmentX Seal and purge with Nitrogen

Technician: VS

Location: NBP

***CTD Pump (Secondary)*****NBP-Bird Electronics, Inc**

53° 10'S, 70° 50'W, Punta Arenas, Chile

Phone: (808)434-9769, (808)659-5076 Fax: 011-870-336-661-014

Email: et@NBP.usap.gov

**SBE 5+ Pump Service & Calibration**

4/27/08

S/N 051627

X Check all O-rings, lubricate and install new O-rings if requiredX Check Thrust Washers, replace if necessaryX Remove and clean impeller – reinstallX Tune R11 as necessary for RPM adjustmentX Seal and purge with Nitrogen

Technician: VS

Location: NBP

## CTD Dissolved Oxygen (Primary)

**SEA-BIRD ELECTRONICS, INC.**  
**1808 136th Place N.E., Bellevue, Washington, 98005 USA**  
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com


SENSOR SERIAL NUMBER: 0139  
 CALIBRATION DATE: 21-Apr-09p

SBE 43 OXYGEN CALIBRATION DATA

COEFFICIENTS	A = -1.2634e-003	NOMINAL DYNAMIC COEFFICIENTS
Soc = 0.3782	B = 1.4686e-004	D1 = 1.92634e-4 H1 = -3.30000e-2
Voffset = -0.5940	C = -3.3967e-006	D2 = -4.64803e-2 H2 = 5.00000e+3
Tau20 = 1.13	E nominal = 0.036	H3 = 1.45000e+3

BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.25	2.00	0.00	0.934	1.24	-0.00
1.25	6.00	0.01	0.974	1.25	-0.00
1.25	12.00	0.01	1.033	1.25	0.00
1.26	20.00	0.01	1.117	1.27	0.01
1.26	26.00	0.01	1.182	1.27	0.01
1.27	30.00	0.01	1.230	1.28	0.01
4.12	30.00	0.01	2.652	4.13	0.00
4.13	20.00	0.01	2.298	4.12	-0.00
4.13	6.00	0.01	1.849	4.12	-0.01
4.13	12.00	0.01	2.040	4.13	-0.00
4.14	26.00	0.01	2.307	4.13	-0.00
4.14	2.00	0.00	1.724	4.13	-0.01
6.55	30.00	0.01	3.862	6.55	-0.00
6.66	26.00	0.01	3.673	6.66	-0.01
6.68	20.00	0.01	3.357	6.69	0.00
6.73	12.00	0.01	2.955	6.73	0.00
6.76	6.00	0.01	2.653	6.76	0.00
6.83	2.00	0.00	2.467	6.84	0.01

Oxygen (ml/l) = Soc \* (V + Voffset) \* (1.0 + A \* T + B \* T<sup>2</sup> + C \* T<sup>3</sup>) \* OxSol(T,S) \* exp(E \* P / K)  
 V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU] K = temperature [deg K]  
 OxSol(T,S) = oxygen saturation [ml/l], P = pressure [dbar], Residual = instrument oxygen - bath oxygen

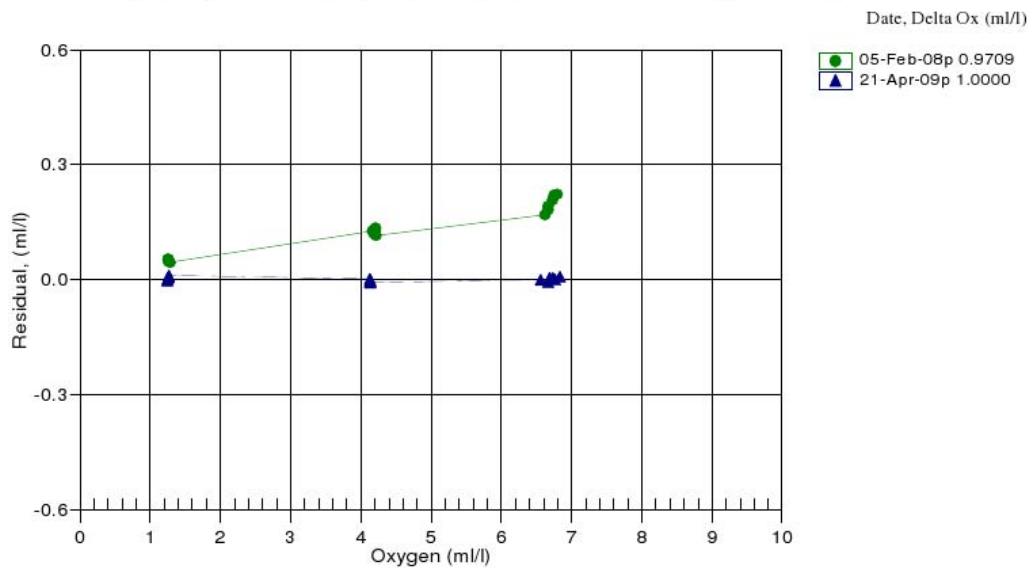

## CTD Dissolved Oxygen (Secondary)

**SEA-BIRD ELECTRONICS, INC.**  
**1808 136th Place N.E., Bellevue, Washington, 98005 USA**  
 Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0155  
 CALIBRATION DATE: 21-Apr-09p

SBE 43 OXYGEN CALIBRATION DATA

COEFFICIENTS	A = -1.9042e-003	NOMINAL DYNAMIC COEFFICIENTS
Soc = 0.3493	B = 2.4147e-004	D1 = 1.92634e-4 H1 = -3.30000e-2
Voffset = -0.4808	C = -4.1242e-006	D2 = -4.64803e-2 H2 = 5.00000e+3
Tau20 = 1.01	E nominal = 0.036	H3 = 1.45000e+3


BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.25	2.00	0.00	0.850	1.25	-0.00
1.25	6.00	0.01	0.893	1.25	0.00
1.25	12.00	0.01	0.954	1.25	0.00
1.26	20.00	0.01	1.030	1.26	0.00
1.26	26.00	0.01	1.094	1.27	0.00
1.27	30.00	0.01	1.130	1.27	0.00
4.12	30.00	0.01	2.607	4.12	-0.00
4.13	20.00	0.01	2.292	4.13	-0.00
4.13	6.00	0.01	1.841	4.12	-0.00
4.13	12.00	0.01	2.040	4.13	-0.00
4.14	26.00	0.01	2.483	4.13	-0.00
4.14	2.00	0.00	1.706	4.13	-0.01
6.55	30.00	0.01	3.864	6.56	0.00
6.66	26.00	0.01	3.709	6.67	0.00
6.68	20.00	0.01	3.413	6.68	-0.00
6.73	12.00	0.01	3.024	6.73	0.00
6.76	6.00	0.01	2.712	6.76	0.00
6.83	2.00	0.00	2.509	6.84	0.00

$$\text{Oxygen (ml/l)} = \text{Soc} * (\text{V} + \text{Voffset}) * (1.0 + \text{A} * \text{T} + \text{B} * \text{T}^2 + \text{C} * \text{T}^3) * \text{OxSol(T,S)} * \exp(\text{E} * \text{P} / \text{K})$$

V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU] K = temperature [deg K]

OxSol(T,S) = oxygen saturation [ml/l], P = pressure [dbar], Residual = instrument oxygen - bath oxygen

Date, Delta Ox (ml/l)

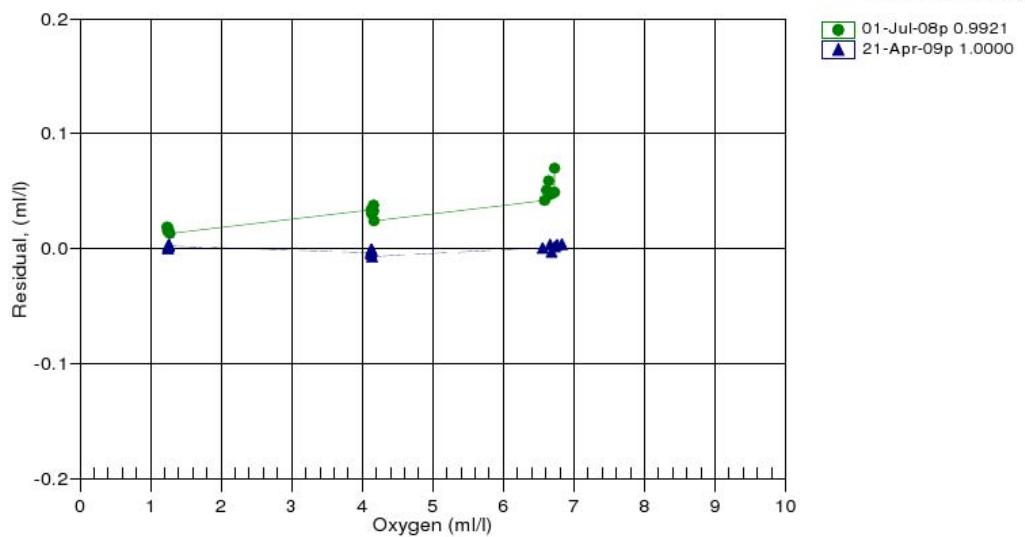

## CTD Fluorometer

PO Box 518  
 620 Applegate St.  
 Philomath OR 97370

**Labs**

(541) 929-5650  
 Fax (541) 929-5277  
<http://www.wetlabs.com>

**Chlorophyll Fluorometer Characterization**

**Date:** 02/24/09  
**Serial #:** AFL-016D  
**Job#:** 0102007  
**Tech:** K.C

<b>Dark Counts</b>	<b>0.164 volts</b>
<b>CEV</b>	<b>2.092 volts</b>
<b>SF</b>	<b>10.6327</b>
<b>FSV</b>	<b>5.45 volts</b>
<b>Linearity:</b>	<b>0.999 R<sup>2</sup> (0–1.5 volts)</b>
	<b>0.995 R<sup>2</sup> (0–5.45 volts)</b>

Notes:

**Dark Counts:** Signal output of the meter in clean water with black tape over detector.

**CEV** is the chlorophyll equivalent voltage. This value is the signal output of the fluorometer when using a fluorescent proxy that has been determined to be approximately equivalent to 25 µg/l of a *Thalassiosira weissflogii* phytoplankton culture.

**SF** is the scale factor used to derive chlorophyll concentration from the signal voltage output of the fluorometer. The scale factor is determined by using the following equation:  
 $SF = (25) / (CEV - \text{dark})$  e.g.  $(25 / (2.865 - 0.238)) = 9.516$

**FSV** is the maximum signal voltage output that the fluorometer is capable of.

Chlorophyll concentration expressed in µg/l (mg/m<sup>3</sup>) can be derived by using the following equation: ( $\mu\text{g/l}$ ) = ( $V_{\text{measured}} - \text{dark}$ ) \* SF

The relationship between fluorescence and chlorophyll-a concentrations in-situ is highly variable. The scale factor listed on this document was determined by using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer you must perform secondary measurements on the populations of interest. This is typically done using extraction based measurement techniques on discrete samples. For additional information on determination of chlorophyll concentration see [Standard Methods For The Examination Of Water And Wastewater] part 10200 H published jointly by: American Public Health Association, American Water Works Association and Water Environment Federation.

**CTD Transmissometer**

PO Box 518  
620 Applegate St.  
Philomath, OR 97370



(541) 929-5650  
Fax (541) 929-5277  
[www.wetlabs.com](http://www.wetlabs.com)

**C-Star Calibration**

Date	April 9, 2008	S/N#	CST-802DR	Pathlength	25 cm
------	---------------	------	-----------	------------	-------

**Analog meter**

$V_d$	0.061 V
$V_{air}$	4.884 V
$V_{ref}$	4.768 V

Temperature of calibration water	23.3 °C
Ambient temperature during calibration	25.1 °C

Relationship of transmittance (Tr) to beam attenuation coefficient (c), and pathlength (x):  $Tr = e^{-cx}$

To determine beam transmittance:  $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient:  $c = -1/x * \ln(Tr)$

$V_d$  Meter output with the beam blocked. This is the offset.

$V_{air}$  Meter output in air with a clear beam path.

$V_{ref}$  Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain  $V_{ref}$ .

Ambient temperature: meter temperature in air during the calibration.

$V_{sig}$  Measured signal output of meter.

**CTD PAR**

Biospherical Instruments Inc																																																																																																	
CALIBRATION CERTIFICATE																																																																																																	
UNDERWATER PAR SENSOR WITH LOG AMPLIFIER																																																																																																	
Calibration Date:	10/16/08			Job No.:	R-10029																																																																																												
Model Number:	QSP-200L																																																																																																
Serial Number:	4361																																																																																																
Operator:	TPC																																																																																																
Standard Lamp:	91537(10/25/06)																																																																																																
Operating Voltage Range:	6	to	15	VDC (+)																																																																																													
Note: The QSP-200 uses a log amplifier to measure the detector signal current with $V = \log I$ (Amps) / $I_{Ref}$																																																																																																	
To calculate irradiance, use this formula:																																																																																																	
$Irradiance = Calibration factor * (10^V_{Light} - 10^{V_{Dark}})$																																																																																																	
With the appropriate (solar corrected) Irradiance Calibration Factor:																																																																																																	
Dry Calibration Factor:	5.26E+12	quanta/cm <sup>2</sup> ·sec/"amps"	8.74E-06	μEinsteins/cm <sup>2</sup> ·sec/"amps"																																																																																													
Wet Calibration Factor:	8.86E+12	quanta/cm <sup>2</sup> ·sec/"amps"	1.47E-05	μEinsteins/cm <sup>2</sup> ·sec/"amps"																																																																																													
<b>Sensor Test Data and Results<sup>4)</sup></b>																																																																																																	
<table border="1"> <thead> <tr> <th colspan="2">Sensor Supply Current (Dark):</th> <th>76.6</th> <th>mA</th> <th colspan="5"></th> </tr> <tr> <th colspan="2">Supply Voltage:</th> <td>6</td> <td>Volts</td> <th colspan="5"></th> </tr> <tr> <th colspan="2">Lamp Integrated PAR Irradiance:</th> <td>8.83E+15</td> <td>quanta/cm<sup>2</sup>·sec</td> <td>0.01467</td> <td>μEinsteins/cm<sup>2</sup>sec</td> <th colspan="3"></th> </tr> <tr> <th>Nominal Filter OD</th> <th>Calibrated Trans.</th> <th>Sensor Voltage</th> <th>Measured Trans.</th> <th>Measured Signal (Amps)</th> <th>Estimated Signal (Amps)</th> <th>Calc. Output (Volts)</th> <th>Error (Volts)</th> <th>Test Irrad. (quanta/cm<sup>2</sup>·sec)</th> </tr> </thead> <tbody> <tr> <td>No Filter</td> <td>100.00%</td> <td>3.226</td> <td>100.00%</td> <td>1.68E-07</td> <td>1.68E-07</td> <td>3.226</td> <td>0.000</td> <td>0.0</td> </tr> <tr> <td>0.3</td> <td>36.10%</td> <td>2.782</td> <td>35.91%</td> <td>6.04E-08</td> <td>6.07E-08</td> <td>2.784</td> <td>0.003</td> <td>0.5</td> </tr> <tr> <td>0.5</td> <td>27.60%</td> <td>2.669</td> <td>27.66%</td> <td>4.65E-08</td> <td>4.64E-08</td> <td>2.668</td> <td>-0.001</td> <td>-0.2</td> </tr> <tr> <td>1</td> <td>9.27%</td> <td>2.206</td> <td>9.47%</td> <td>1.59E-08</td> <td>1.56E-08</td> <td>2.197</td> <td>-0.009</td> <td>-2.2</td> </tr> <tr> <td>2</td> <td>1.11%</td> <td>1.320</td> <td>1.15%</td> <td>1.93E-09</td> <td>1.87E-09</td> <td>1.306</td> <td>-0.014</td> <td>-3.5</td> </tr> <tr> <td>3</td> <td>0.05%</td> <td>0.458</td> <td>0.08%</td> <td>1.30E-10</td> <td>8.98E-11</td> <td>0.393</td> <td>-0.065</td> <td>-30.7</td> </tr> </tbody> </table>								Sensor Supply Current (Dark):		76.6	mA						Supply Voltage:		6	Volts						Lamp Integrated PAR Irradiance:		8.83E+15	quanta/cm <sup>2</sup> ·sec	0.01467	μEinsteins/cm <sup>2</sup> sec				Nominal Filter OD	Calibrated Trans.	Sensor Voltage	Measured Trans.	Measured Signal (Amps)	Estimated Signal (Amps)	Calc. Output (Volts)	Error (Volts)	Test Irrad. (quanta/cm <sup>2</sup> ·sec)	No Filter	100.00%	3.226	100.00%	1.68E-07	1.68E-07	3.226	0.000	0.0	0.3	36.10%	2.782	35.91%	6.04E-08	6.07E-08	2.784	0.003	0.5	0.5	27.60%	2.669	27.66%	4.65E-08	4.64E-08	2.668	-0.001	-0.2	1	9.27%	2.206	9.47%	1.59E-08	1.56E-08	2.197	-0.009	-2.2	2	1.11%	1.320	1.15%	1.93E-09	1.87E-09	1.306	-0.014	-3.5	3	0.05%	0.458	0.08%	1.30E-10	8.98E-11	0.393	-0.065	-30.7
Sensor Supply Current (Dark):		76.6	mA																																																																																														
Supply Voltage:		6	Volts																																																																																														
Lamp Integrated PAR Irradiance:		8.83E+15	quanta/cm <sup>2</sup> ·sec	0.01467	μEinsteins/cm <sup>2</sup> sec																																																																																												
Nominal Filter OD	Calibrated Trans.	Sensor Voltage	Measured Trans.	Measured Signal (Amps)	Estimated Signal (Amps)	Calc. Output (Volts)	Error (Volts)	Test Irrad. (quanta/cm <sup>2</sup> ·sec)																																																																																									
No Filter	100.00%	3.226	100.00%	1.68E-07	1.68E-07	3.226	0.000	0.0																																																																																									
0.3	36.10%	2.782	35.91%	6.04E-08	6.07E-08	2.784	0.003	0.5																																																																																									
0.5	27.60%	2.669	27.66%	4.65E-08	4.64E-08	2.668	-0.001	-0.2																																																																																									
1	9.27%	2.206	9.47%	1.59E-08	1.56E-08	2.197	-0.009	-2.2																																																																																									
2	1.11%	1.320	1.15%	1.93E-09	1.87E-09	1.306	-0.014	-3.5																																																																																									
3	0.05%	0.458	0.08%	1.30E-10	8.98E-11	0.393	-0.065	-30.7																																																																																									
<table border="1"> <thead> <tr> <th>Dark Before:</th> <th>0.197</th> <th>Volts</th> <th><math>I_{Ref} = 1.00E-10</math> Amps</th> <th colspan="4"></th> </tr> <tr> <th>Light - No Filter Hldr.:</th> <th>3.225</th> <th>Volts</th> <th><math>I_{Dark} = 1.58E-10</math> Amps</th> <th colspan="4"></th> </tr> <tr> <th>Dark After - NFH:</th> <th>0.199</th> <th>Volts</th> <th><math>10^{V_{Dark}} = 1.576703</math> Amps</th> <th colspan="4"></th> </tr> <tr> <th>Average Dark</th> <th>0.198</th> <th>Volts</th> <th>RG780</th> <th colspan="4">1.023</th> </tr> </thead> <tbody> <tr> <td colspan="8">Notes:</td> </tr> <tr> <td colspan="8">Annual calibration is recommended.</td> </tr> <tr> <td colspan="8">There is increasing error associated with readings below zero.</td> </tr> <tr> <td colspan="8">The collector should be cleaned frequently with alcohol.</td> </tr> <tr> <td colspan="8">This section is for internal use and for more advanced analysis.</td> </tr> </tbody> </table>								Dark Before:	0.197	Volts	$I_{Ref} = 1.00E-10$ Amps					Light - No Filter Hldr.:	3.225	Volts	$I_{Dark} = 1.58E-10$ Amps					Dark After - NFH:	0.199	Volts	$10^{V_{Dark}} = 1.576703$ Amps					Average Dark	0.198	Volts	RG780	1.023				Notes:								Annual calibration is recommended.								There is increasing error associated with readings below zero.								The collector should be cleaned frequently with alcohol.								This section is for internal use and for more advanced analysis.																									
Dark Before:	0.197	Volts	$I_{Ref} = 1.00E-10$ Amps																																																																																														
Light - No Filter Hldr.:	3.225	Volts	$I_{Dark} = 1.58E-10$ Amps																																																																																														
Dark After - NFH:	0.199	Volts	$10^{V_{Dark}} = 1.576703$ Amps																																																																																														
Average Dark	0.198	Volts	RG780	1.023																																																																																													
Notes:																																																																																																	
Annual calibration is recommended.																																																																																																	
There is increasing error associated with readings below zero.																																																																																																	
The collector should be cleaned frequently with alcohol.																																																																																																	
This section is for internal use and for more advanced analysis.																																																																																																	
QSP-200L,QSP2300(2006- ) .xls																																																																																																	