

LMG 1603 Palmer Turnover

Cruise Data Report W. Kevin Pedigo

29 Mar, 2016 – 13 Apr, 2016

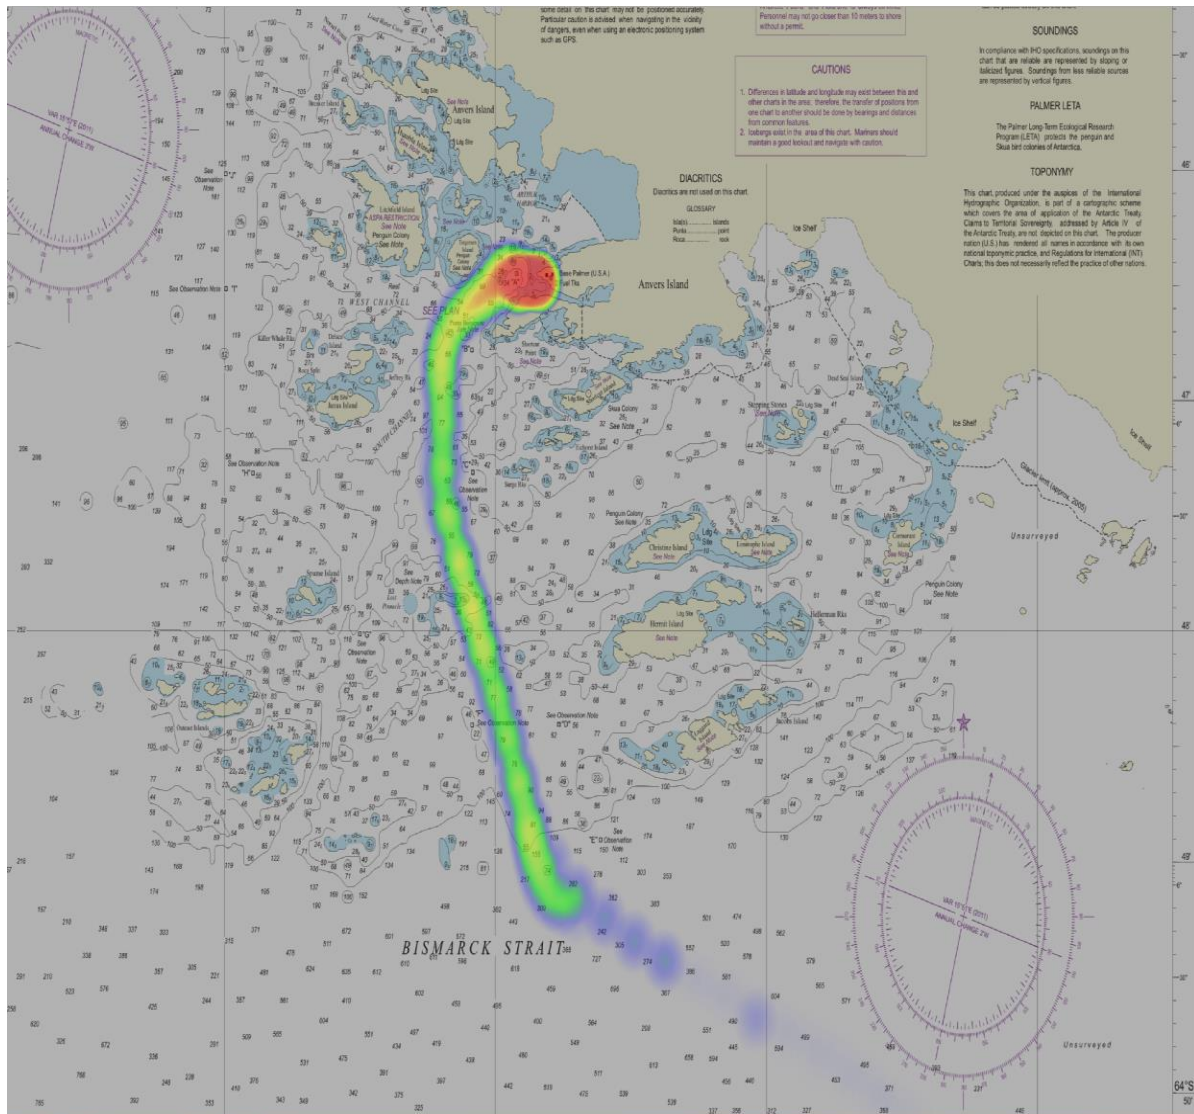


Table of Contents

Table of Contents

LMG 1603 PALMER TURNOVER	1
CRUISE DATA REPORT	1
INTRODUCTION	1
ARCHIVE DATA EXTRACTION	2
DISTRIBUTION CONTENTS	3
ADCP DATA (/ADCP)	3
DATA COLLECTION PARAMETERS (/CAL)	3
IMAGERY (/IMAGERY).....	3
MAPS (/MAPS)	3
OCEAN DATA (/OCEAN).....	3
AUTOMATICALLY PROCESSED DATA (/PROCESS).....	3
REPORTS (/REPORT).....	3
INSTRUMENT DATA (/RVDAS)	3
UTILITY PROGRAMS (/UTILITY)	3
JGOFS DATA SET	4
PCO2-MERGED DATA SET	5
RVDAS	6
SENSORS AND INSTRUMENTS	6
UNDERWAY SENSORS	7
<i>Meteorological Data</i>	7
<i>Navigational Data</i>	7
<i>Geophysical Data</i>	7
<i>Oceanographic Data</i>	7

DATA FILE NAMES AND STRUCTURES	8
LKNL – KNUDSEN CHIRP 3260 SONAR	9
LWN1 - WINCHES	9
LMWX – CAMPBELL METEOROLOGICAL DAS	10
LSEA – WET WALL FLOWS, TRANSMISSOMETER	11
UTSG – MICROTSG, THERMOSALINOGRAPH	12
LRTM – DIGITAL REMOTE TEMPERATURE	12
LDL – FLUOROMETER, WETLAB ECO	12
LGO2 – OXYGEN SYSTEM	13
LOXY – OXYGEN (PART OF PCO2 SYSTEM, SEPARATE FROM OXYGEN SYSTEM)	15
LPCO – PCO2 SYSTEM	16
LSVP - SOUND VELOCITY PROBE IN ADCP TRANSDUCER WELL	17
LADC – ADCP SPEED LOG	17
LGYR - GYROCOMPASS	18
LSEP – SEAPATH 330 GPS	18
LGAR - GARMIN GPS	22
LAIS – AIS RECEIVER	24
LMG SENSORS	25
SHIPBOARD SENSORS	25
UNDERWAY CALIBRATION SHEETS	26
ACQUISITION AND PROCESSING INFORMATION	41
ERRORS AND EVENTS	41
INTRODUCTION	1
ARCHIVE DATA EXTRACTION	2
DISTRIBUTION CONTENTS	3
ADCP DATA (/ADCP)	3

DATA COLLECTION PARAMETERS (/CAL)	3
IMAGERY (/IMAGERY).....	3
MAPS (/MAPS)	3
OCEAN DATA (/OCEAN).....	3
AUTOMATICALLY PROCESSED DATA (/PROCESS).....	3
REPORTS (/REPORT).....	3
INSTRUMENT DATA (/RVDAS)	3
UTILITY PROGRAMS (/UTILITY)	3
JGOFS DATA SET	4
PCO2-MERGED DATA SET	5
RVDAS	6
SENSORS AND INSTRUMENTS	6
UNDERWAY SENSORS	7
<i>Meteorological Data</i>	7
<i>Navigational Data</i>	7
<i>Geophysical Data</i>	7
<i>Oceanographic Data</i>	7
DATA FILE NAMES AND STRUCTURES	8
LKNV – KNUDSEN CHIRP 3260 SONAR	9
LWN1 - WINCHES	9
LMWX – CAMPBELL METEOROLOGICAL DAS	10
LSEA – WET WALL FLOWS, TRANSMISSOMETER.....	11
UTSG – MICROTSR, THERMOSALINOGRAPH	12
LRTM – DIGITAL REMOTE TEMPERATURE.....	12
LDL – FLUOROMETER, WETLAB ECO	12
LGO2 – OXYGEN SYSTEM	13
LOXY – OXYGEN (PART OF PCO2 SYSTEM, SEPARATE FROM OXYGEN SYSTEM)	15

LPCO – PCO2 SYSTEM	16
LSVP - SOUND VELOCITY PROBE IN ADCP TRANSDUCER WELL.....	17
LADC – ADCP SPEED LOG	17
LGYR – GYROCOMPASS	18
LSEP – SEAPATH 330 GPS.....	18
LGAR - GARMIN GPS	22
LAIS – AIS RECEIVER	24
LMG SENSORS.....	25
SHIPBOARD SENSORS.....	25
UNDERWAY CALIBRATION SHEETS	26
ACQUISITION AND PROCESSING INFORMATION.....	41
ERRORS AND EVENTS.....	41

Introduction

The LMG data acquisition systems continuously log data from a suite of instrumentation throughout the cruise. This document describes:

- The structure and organization of the data on the distribution media
- The format and contents of the data strings
- Formulas for calculating values
- Information about the specific instruments in use during the cruise
- A log of acquisition problems and events during the cruise that may affect the data
- Scanned calibration sheets for the instruments in use during the cruise.

All the data has been archived using 'tar' and compressed using 'gzip', identified by the '.tz' extension. Tools are available on all platforms for uncompressing and de-archiving these formats: On Macintosh use the built-in Archive Utility, or tar in the terminal. On Windows operating systems use WinZip or 7Zip.

IMPORTANT: Read the last section, "Acquisition Problems and Events," for important information that may affect the processing of this data.

Archive Data Extraction

It is often useful to know exactly how an archive was produced when expanding its contents. Tar files were created using the following commands:

```
tar cvf archive-file files-to-be-archived
```

To create a list of the files in the archive:

```
tar tvf archive-file > contents.list
```

To extract the files from the archive:

```
tar xvf archive-file file(s)-to-extract
```

G-zipped files will have a “.gz” extension on the filename. These files can be decompressed after de-archiving, using:

```
gunzip filename.gz
```

Distribution Contents

ADCP data (/ADCP)

This directory contains a tar file of the ADCP system's "proc" directory, which contains a database of the averaged ping data, Matlab m-files used in processing the data, and daily graphs of the currents. For more information contact Teri Chereskin at tchereskin@ucsd.edu.

Data collection parameters (/CAL)

Refer to the InstCoef.txt file along with the specific instrument calibration sheets in this report for information on how the RVDAS data was collected and processed.

Imagery (/Imagery)

This directory contains things such as ice imagery, isobar charts, sat imagery, wave and wind images, and weather reports.

Maps (/Maps)

This directory maps and mapping data generated by the ship's MCIS and automated scripts, plus any maps provided for this purpose by the on-board science party.

Ocean data (/ocean)

This directory will contain data on XBT's, XCTD's, and CTD's deployed.

Automatically processed data (/process)

Contains automatically processed datasets and QC graphs produced by the RVDAS system

Reports (/Report)

Copies of this report in MS Word and pdf formats, and scanned copies of logsheets provided by various science groups.

Instrument data (/rvdas)

Contains data collected by the suite of standard instruments on the LMG.

Utility programs (/Utility)

Contains utility programs to access the data on the distribution.

JGOFS Data Set

/Process/JGOF/

The JGOFS data set consists of a single file produced each day named jg<julian_day>.dat.gz where <julian_day> is the day the data was acquired. The “.gz” extension indicates that the individual files are compressed before archiving. The daily file consists of 22 separate columnar fields in text format, which are described below. The JGOFS data set is obtained primarily by applying calibrations to raw data and decimating to whole minute intervals. However, several fields are derived measurements from more than a single raw input. *Note: Null, unused, or unknown fields are filled with 9's in the JGOFS data.*

Additionally, 3 separate QC plots are generated daily by the ET using the JGOFS data set. These plots include TSG and Bathymetry data, meteorological data, and navigation data. The files are called ocean<julian_day>.ps, met<julian_day>.ps, and nav<julian_day>.ps respectively.

Field	Data	Units
01	GMT Date	dd/mm/yy
02	GMT Time	hh:mm:ss
03	Seapath Latitude (negative is South)	tt.tttt
04	Seapath Longitude (negative is West)	ggg.gggg
05	Speed Over Ground	knots
06	GPS HDOP	-
07	Gyro Heading	Degrees (azimuth)
08	Course Made Good	Degrees (azimuth)
09	Mast PAR	μEinstein's/meter ²
10	Sea Surface Temperature	°C
11	Sea Surface Conductivity	siemens/meter
12	Sea Surface Salinity	PSU
13	Sea Depth (uncorrected, calc. sw soud vel. 1500 m/s)	meters
14	True Wind Speed (max speed windbird)	meters/sec
15	True Wind Direction (max speed windbird)	degrees (azimuth)
16	Ambient Air Temperature	°C
17	Relative Humidity	%
18	Barometric Pressure	mBars
19	Sea Surface Fluorometry	μg/l
20	Transmissometry	%
21	PSP	W/m ²
22	PIR	W/m ²

pCO₂-merged Data Set

/Process/PCO2/

00+346:23:58:20.672 2000346.9991 2398.4 1008.4 0.01 45.4 350.3 342.6 15.77 Equil -43.6826
 173.1997 15.51 33.90 0.33 5.28 9.05 1007.57 40.0 14.87 182.44 -1

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	pCO ₂ time tag*	yyyyddd.ttt	UTC
3	Raw Voltage (IR)	xxxx.xx	mV
4	Cell Temperature	xx.xx	°C
5	pCO ₂ system internal Barometer	xxx.xx	mBar
6	Flowrate	xxx.xx	cm ³ /min
7	VCO ₂ Concentration	xxx.xx	µAtm
8	pCO ₂ Pressure	xx.xx	ppm
9	Equilibrator Temperature, RTD	xx.xx	°C
10	Equilibrator Temperature, SBE38	xx.xx	°C
11	Valve Position	xx	numeric
12	Gas Flow Source (Equil = pCO ₂ measurement)		text
13	Latitude	xx.x	degrees
14	Longitude	xxx.xxxxx	degrees
15	Sea Water Intake Temperature	xx.xxx	°C
16	Sea Surface Salinity	xx.xxx	PSU
17	Sea Surface Fluorometry	x.xxx	mg/m ³
18	True Wind Speed	x.xx	m/s
19	True Wind Direction	x.xx	degrees
20	Barometric Pressure	xxx.xx	mBar
21	Hydro-Lab H ₂ O Flow Rate	xxx.x	Raw counts
22	Speed over Ground	x.xx	knots
23	Course Made Good	xx.xx	degrees
24	Oxygen	xxx.xx	µm/kg
25	TSG2 Internal Temperature	x.xx	°C
26	TSG2 Salinity	xx.xx	PSU
27	TSG1 Internal Temperature	x.xx	°C

RVDAS

/RVDAS/

RVDAS (Research Vessel Data Acquisition System) was developed at Lamont-Doherty Earth Observatory of Columbia University and was used on the R/V Maurice Ewing for many years. It was extensively for use on the Nathaniel B. Palmer and her sister ship, the R/V Laurence M. Gould.

Daily data processing of the RVDAS data is performed to calibrate and convert values into useable units and as a quality-control on operation of the DAS. Raw and processed data sets from RVDAS are included in the data distribution. The tables below provide detailed information on the sensors and data. Be sure to read the “Significant Acquisition Events” section for important information about data acquisition during this cruise.

Sensors and Instruments

RVDAS data is divided into two general categories, *underway and navigation*. They can be found on the distribution media as subdirectories under the top level `rvdas` directory: `/rvdas/uw`, and `/rvdas/nav`. Processed oceanographic data is in the top level directory, `/process`. Each instrument or sensor produces a data file named with its channel ID. Each data file is g-zipped to save space on the distribution media. Not all data types are collected every day or on every cruise.

The naming convention for data files produced by the sensors and instruments is

`LMG[CruiseID] [ChannelID] .dDDD`

Example: `LMG1603lmwx.d025`

- The CruiseID is the numeric name of the cruise, in this case, `1603`.
- The ChannelID is a 4-character code representing the system being logged. An example is “mw1,” the designation for meteorology.
- DDD is the day of year the data was collected

Underway Sensors

Meteorological Data

Measurement	String ID	Collection Status	Rate	Instrument
Air Temperature	lmwx (met)	Continuous	1/sec	RM Young 41372LC
Relative Humidity	lmwx (met)	Continuous	1/sec	RM Young 41372LC
Wind Speed / Direction	lmwx (pus,sus)	Continuous	1/sec	Gill Instruments 1390-PK-062
Barometer	lmwx (met)	Continuous	1/sec	Vaisala PTB210B
PAR	lmwx (met)	Continuous	1/sec	Biospherical Instruments QSR-240
PIR	lmwx (met)	Continuous	1/sec	Eppley PIR
PSP	lmwx (met)	Continuous	1/sec	Eppley PSP
GUV	lguv	Continuous	2/sec	Biospherical Instruments GUV-2511
Oxygen	lgo2	Continuous	1/min	UCAR Oxygen system

Navigational Data

Measurement	String ID	Collection Status	Rate	Instrument
Gyroscope	lgyr	Continuous	5/sec	Meridian Bridgmate Gyro
Seapath GPS	lsep	Continuous	1/sec	Seapath 330
Garmin GPS	lgar	Continuous	1/sec	Garmin 17
AIS	lais	Continuous	var	Standard Horizon GX2150

Geophysical Data

Measurement	String ID	Collection Status	Rate	Instrument
Bathymetry	lknu	Variable	Varies	Knudsen Chirp 3260
Dush-11 Winch	lwn1	Variable	20/sec	Markey DUSH-11
Dush-5 Winch	lwn1	Variable	20/sec	Markey DUSH-5
Dush-4 Winch	lwn1	Variable	20/sec	Markey DUSH-4

Oceanographic Data

Measurement	String ID	Collection Status	Rate	Instrument
Salinity	utsg	Continuous	3 sec	Seabird-45
Salinity (secondary)	tsg2	Continuous	3 sec	Seabird-45
Sea Surface Temperature	lrtm	Continuous	1 sec	Seabird-38
Fluorometry	ldfl	Continuous	1 sec	WetLabs ECO
ADCP, Speed Log	ladc	Continuous	1 sec	RD Instruments Workhorse 150
Dissolved Oxygen	loxy	Continuous	1 sec	Anderaa Optode
pCO ₂	lpco2	Continuous	2.5 min	PCO2 System

Data File Names and Structures

RVDAS data is divided into two broad categories, **Underway** and **Navigation**. The groups are abbreviated “uw” and “nav”. Thus, these two tar files, lmguw.tar and lmgnav.tar exist under the top-level rvdas directory. The instruments are broken down as shown. Each data file is g-zipped to save space on the distribution. Not all data types are collected every day or on every cruise.

RVDAS data files are named following the convention: LMG[FileID].dDDD.

- The FileID is a 4-character code representing the system being logged, for example: lmet (for meteorology)
- DDD is the Julian day of the data collection

Underway Data	File ID	Navigation Data	File ID
Meteorological	lmtx	Gyro Compass	lgyr
Knudsen	lknu	Garmin GPS	lgar
microTSG	utsg	Seapath GPS	lsep
Sea Surface Temperature	lrtm	AIS	lais
Fluorometer	ldfl		
ADCP	ldfl		
Sound Velocity Probe	lsvp		
GUV & PUV	lguv		
PCO2 system	lpco		
Dissolved Oxygen	loxy		
Sea Water Wall	lsea		
Winches	lwn1		
Net Depth Sensor	lnds		

Data is received by the RVDAS system via RS-232 serial connections. The data files that comprise the rvdas data set are described below. A time tag is added to each line of data received and the data is written to disk.

```
YY+DDD:HH:MM:SS.SSS [data stream from instrument]
```

Where, YY: two-digit year, DDD: Julian Day, HH: 2 digit hours, MM: 2 digit minutes SS.SSS: seconds. All times are UTC.

The delimiters used to separate fields in the raw data files are usually spaces and commas, but other delimiters are used (:, =, @) and occasionally there is no delimiter. Care should be taken when reprocessing the data that the field separations are clearly understood. Example data strings of the loggers follow.

lknu – Knudsen Chirp 3260 Sonar

14+002:19:07:04.648 3.5kHz,4000.92,1,12.0kHz,4001.12,1,1500,-57.343073,-63.750720

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	3.5kHz = Low frequency in use	text	3.5kHz
3	Low Frequency Depth	xxxx.xx	m
4	Valid Flag	x	0 or 1
5	12.0kHz = High frequency in use	text	12.0kHz
6	High Frequency Depth	xxxx.xx	m
7	Valid Flag	x	0 or 1
8	Sound Speed Velocity	xxxx	m/s
9	Latitude	xx.xxxxxx	degrees
10	Longitude	xx.xxxxxx	degrees

lwn1 - Winches

16+093:16:55:49.561 -01RD,2016-04-02T12:38:50.854,DUSH11,-0000233,00000000,000000.0,3275

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Record Identifier, RD=Remote Data		alphanumeric
3	LCI-90i Date and Time	yyyy-mm-ddThh:mm:ss	
4	Winch Identifier		text
5	Winch Name		alphabetical
6	Tension	xxxxxxxx	lbs
7	Speed	xxxxx.x	m/min
8	Payout	xxxxx.x	m
9	Checksum	x.xxxx	numeric

Imwx – Campbell Meteorological DAS

08+034:13:52:14.454 MET, 12.22322, 44.25706, -75, -25, -363.6365, 2.332982, -0.08215196, 278.6845, 279.2192, 854.6198, 854.6184

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	MET Flag		
3	Power Supply Voltage	vv.v	V
4	Enclosure Relative Humidity (not implemented)	xx.x	%
5	Air Temperature, Celsius	xx.x	C
6	Air Relative Humidity	xx.x	%
7	PAR (Photosynthetically Available Radiation)	xxx.xxxx	mV
8	PSP (Shortwave Radiation)	x.xxxxxx	mV
9	PIR Thermopile (Longwave Radiation)	x.xxxxxx	mV
10	PIR Case Temperature	xxx.xxxx	K
11	PIR Dome Temperature	xxx.xxxx	K
12	Barometer	xxx.xxxx	mBar
13	Secondary Barometer (experimental)	xxx.xxxx	mBar

08+034:13:52:14.216 PUS, A, 356, 002.15, M, +332.28, +000.97, 60, 08

08+034:13:52:14.216 SUS, A, 356, 002.15, M, +332.28, +000.97, 60, 08

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Identifier (PUS = port, SUS = stbd)	xxx	Text
3	A	x	A
4	Port Wind Relative Direction	xxx	degrees
5	Port Wind Relative Speed	xxx.xx	m/s
6	M = Meters (for previous)	x	M
7	Sound Speed	xxx.xx	m/s
8	Sonic Temperature	xxx.xx	°C
9	Unit Status	xx	numeric
10	Checksum	xx	alphanumeric

Isea – wet wall flows, transmissometer

12+004:12:01:04.438 WetLab_1,14.1,XMISS,3.098,V,0.000,0.000,0.000,-928.535,-
 220.566,0.000,0.000,T,NAN,NAN,NAN,NAN,P,0,0,F,47.91811,0,6.815308,0,0,0,0,0,I,1,1,1,1

Field	Data	Unit
1	RVDAS time tag	UTC
2	WetLat_1	Text
3	Internal Temperature	°C
4	XMISS	Text
5	Transmissometer Reading	volts
6	V	Text
7	High precision voltage #1	V
8	High precision voltage #2	V
9	High precision voltage #3	V
10	Standard precision voltage #1 (historically used for YoYo Cam xmiss)	V
11	Standard precision voltage #2 (historically used for YoYo Cam altimeter)	V
12	Standard precision voltage #3	V
13	Standard precision voltage #4	V
14	T	Text
15	Temperature Probe 1	°C
16	Temperature Probe 2	°C
17	Temperature Probe 3	°C
18	Temperature Probe 4	°C
19	P	Text
20	Pulse Counter 1	counts
21	Pulse Counter 2	counts
22	F	Text
23	Flow Counter #1	counts
24	Flow Counter #2	counts
25	Flow Counter #3	counts
26	Flow Counter #4	counts
27	Flow Counter #5	counts
28	Flow Counter #6	counts
29	Flow Counter #7	counts
30	Flow Counter #8	counts
31	I	Text
32	Digital Input #1	1 or 0
33	Digital Input #2	1 or 0
34	Digital Input #3	1 or 0
35	Digital Input #4	1 or 0

utsg – microTSG, Thermosalinograph

For further information on this data, check www.seabird.com for SBE 45 MicroTSG Thermosalinograph

08+037:13:45:57.596 2.6470, 3.03853, 33.8129, 1459.351

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Internal water temperature	xx.xxxx	C
3	Conductivity	xx.xxxx	s/m
4	Salinity	xx.xxxx	PSU
5	Sound Velocity	xxxx.xxx	m/s

lrtm – digital Remote Temperature

For further information on this data, check on www.seabird.com on SBE38 Digital Thermometer

08+037:13:47:17.841 2.2527

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Temperature, Seawater Intake	xx.xxxx	C

ldfl – Fluorometer, Wetlab ECO

08+037:13:55:08.434 99/99/99 99:99:99 0.00 2585 73 543

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Fluorometer Date	mm/dd/yy	text
3	Fluorometer Time	hh:mm:ss	text
4	Chlorophyl Signal	x.xx	µg/l
5	Reference	xxxx	λq
6	Counts – Chlorophyll Signal	xx	counts
7	Thermistor Counts	xxxx	counts

Igo2 - Oxygen System

For further information on this data, please contact Britt Stephens at stephens@ucar.edu

```
12+301:22:35:30.558 81300.8 16.0 32.0 000.0 005.0 1.2589631 1.2379622 744.549 111.853 131.642
-2.089 -2.448 723.594 002.50 086.43 099.74 002.77 000.97 050.65 0.000 001.19 065.59 039.48
1966.097 01.345 37.0171 37.8433 000.0 000.0 20.66 20.41 -92.0 28.66 37.44 42.33 37.80 47.95
0.0 01.88 0.0001711 0.0001712 0.0000747 0.0000725 02.657 02.678 -1 0.0000895 -043.94
```

Field Data

01	RVDAS Time Tag
02	jsecoday - Seconds since midnight
03	jselflag - 8 bit decimal value indicated selected gases
04	jprgflag - 8 bit decimal value indicated purged gases
05	jmfclag - 8 bit decimal value indicated mass-flow controller states
06	jgenflag - 8 bit decimal value indicated other parameters
07	jfcv1 - voltage on Fuel Cell #1
08	jfcv2 - voltage on Fuel Cell #2
09	jpfccl - pressure in torr at fuel cells
10	jlico2a - CO2 in ppm in Li7000 Cell A
11	jlico2b - CO2 in ppm in Li7000 Cell B [CO2 MEASUREMENT]
12	jlih2oa - H2O in ppt in Li7000 Cell A
13	jlih2ob - H2O in ppt in Li7000 Cell B
14	jlipb - pressure in torr at Li7000 Cell B
15	flmfcset - mass-flow controller set voltage
16	jfl1 - flow in sccm on Inlet Line #1
17	jfl2 - flow in sccm on Inlet Line #2
18	jfl1t - flow in sccm on Long-Term reference cylinder
19	jflcal - flow in sccm on selected Calibration cylinder
20	jflwta - flow in sccm on selected Working Tank Cylinder
21	jvsoset - purge line voltage-sensitive orifice set voltage
22	jflpurge - flow in sccm on purge line
23	jflwtb - flow in sccm on Working Tank line through sensors
24	jflsp - flow in sccm on Span line through sensors
25	jpfridge - pressure in torr inside fridge trap
26	jtfridge - temperature in C inside fridge trap
27	jtmpt - fuel-cell control temperature (thermistor) in C for MPT10000
28	jtfcell - fuel-cell thermistor temperature in C
29	jtach1 - rmp of fan inside Line #1 Inlet
30	jtach2 - rmp of fan inside Line #2 Inlet
31	jtcyl1 - temperature in C from cylinder box RTD #1
32	jtcyl2 - temperature in C from cylinder box RTD #2

33	jtchill - temperature in C from chiller RTD
34	jtamb - temperature in C RTD near Analyzer Box electronics
35	jtomega - Analyzer Box control temperature (RTD) for Omega CNI2332
36	jtu4ch - temperature in C inside USB4CH 24-bit A/D box
37	jtfcrtd - fuel-cell RTD temperature in C
38	jtirga - temperature in C inside Li7000
39	jliflags - Li7000 status flag
40	jlirhsrc - Li7000 source/detector relative humidity
41	jsdfcv1 - standard deviation of 1-Hz Fuel Cell #1 voltage
42	jsdfcv2 - standard deviation of 1-Hz Fuel Cell #2 voltage
43	jslfcv1 - slope of 1-Hz Fuel Cell #1 voltage
44	jslfcv2 - slope of 1-Hz Fuel Cell #2 voltage
45	jsdco2a - standard deviation of 1-Hz Li7000 Cell A CO2 in ppm
46	jsdco2b - standard deviation of 1-Hz Li7000 Cell B CO2 in ppm
47	posneg - flag indicating position of fuel-cell changeover valve
48	jogdeltadiff - amplitude of 3-jog O2 difference-signal [O2 MEASUREMENT]

loxy – Oxygen (Part of PCO2 system, separate from Oxygen System)

For further information on this data, contact Tim Newberger at tim.newberger@noaa.gov

04+117:23:57:23.504 MEASUREMENT 3830 380 Oxygen: 309.95 Saturation:
 83.48 Temperature: -1.35 DPhase: 33.41 BPhase: 32.22 RPhase:
 0.00 BAmp: 262.09 BPot: 163.00 RAmp: 0.00 RawTem.:
 694.92

Field	Data	Units
1	RVDAS Time Tag	
2-4	Measurement ID, Model Number, Serial Number	alphanumeric
5	Oxygen heading	text
6	Oxygen Reading	Raw numeric
7	Saturation heading	text
8	Saturation Reading	Raw numeric
9	Temperature heading	text
10	Water Temperature	°C
11	Dphase heading	text
12	Dphase	Raw numeric
13	Bphase heading	text
14	BPhase	Raw numeric
15	Rphase heading	text
16	Rphase	Raw numeric
17	Bamp heading	text
18	Bamp	Raw numeric
19	Bpot heading	text
20	Bpot	Raw numeric
21	Ramp heading	text
22	Ramp	Raw numeric
23	RawTem heading	text
24	RawTemp	Raw numeric

Ipco – PCO2 system

For further information on this data, contact Tim Newberger at tim.newberger@noaa.gov

02+319:23:59:13.748 2002319.99851 7154.27 26.49 1033.6 325.79 6.74 329.3 53.76
0 Equil

Field	Data	Units
1	RVDAS Time Tag	
2	Julian date file string	Julian
3	IR voltage reading	mV
4	Cell temperature	°C
5	Barometer	millibars
6	Gas flow	mL/min
7	VCO2 dry value	PPM
8	PCO2 wet/Delta value	PPM
9	Equilibrator Temperature from RTD	°C
10	Equilibrator Temperature from SBE-38	°C
11	Solenoid position ID	number
12	Measured gas	name

lsvp - Sound Velocity Probe in ADCP Transducer Well

NOTE: This value does not represent or reflect the sound speed in the ocean, and is for internal use by the ADCP.

00+348:01:59:52.128 177204

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	Raw data counts	xxxx	Integer

ladc - ADCP Speed Log

00+019:23:59:59.099 \$PUHAW,UVH,-1.48,-0.51,250.6

Field	Data	Units
1	RVDAS Time Tag	
2	\$PUHAW	
3	UVH (E-W, N-S, Heading)	
4	Ship Speed relative to reference layer ¹ velocity ² , East vector	knots
5	Ship Speed relative to reference layer ¹ velocity ² , North vector	knots
6	Ship heading	degrees

¹The reference layer is an average velocity measured in a number of depth “bins”. On the LMG, the bins are typically eight meters deep and bins 3-10 define the reference layer. Hence, the reference layer is the water column from 16-80 meters beneath the ship.

²The speed output is water velocity relative to the ship’s hull and is therefore opposite of the actual movement of the ship. For example, if the ship’s heading is due north, the North/South reference layer velocity is likely to be negative (southerly).

Igyr - Gyrocompass

02+315:23:59:58.616 \$HEHDT,287.7,T*25

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$HEHDT		
3	Heading	x.xx	degrees
4	T = True (for previous)	x	T
5	Checksum	xx	alphanumeric

Isep - Seapath 330 GPS**INZDA: Time and Date Data**

10+351:23:59:58.142 \$INZDA,235958.08,17,12,2010,,*78

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$INZDA		
3	Time	hhmmss.ss	UTC
4	Day	dd	UTC
5	Month	mm	UTC
6	Year	yyyy	UTC
7	(empty field)	x	Blank or 0
8	Checksum	xx	alphanumeric

INGGA: Global Positioning Fix Data

10+351:23:59:58.142 \$INGGA,235958.07,6118.168460,S,06008.089527,W,1,12,0.7,22.57,M,17.79,M,,*46

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$INGGA		
3	Time	hhmmss.ss	UTC
4	Latitude in degrees with decimal minutes	ddmm.mmmmmm	degrees
5	North or South (for previous)	x	N or S
6	Longitude in degrees with decimal minutes	ddmm.mmmmmm	ddmm.mmmmmm
7	East or West (for previous)	x	E or W
8	GPS quality indicator	x	0 – 6
9	Number of satellites in use (00-99)	xx	00-99
10	Horizontal dilution of precision (HDOP)	x.x	
11	Antenna height	x.xx	meters
12	M = meters (for previous)	X	M
13	Geoidal separation	x.xx	meters
14	M = meters (for previous)	X	M
15	Age of DGPS corrections (null with no DGPS)	x.x	seconds
16	If used, ID of DGPS reference station	Xxxx	0000 - 1023

INRMC: Recommended Minimum Specific GNSS Data

10+351:23:59:58.200 \$INRMC,235958.07,A,6118.168460,S,06008.089527,W,12.8,331.22,171210,11.3,E,A*1C

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$INRMC		
3	Time	hhmmss.sss	UTC
4	Status A=valid data, N=receiver warning	x	A or N
5	Latitude	ddmm.mmmmmm	degrees
6	North or South (for previous)	x	N or S
7	Longitude	ddmm.mmmmmm	degrees
8	East or West (for previous)	x	E or W
9	Speed over Ground, True	x.x	knots
10	Course over Ground True	x.xx	degrees
11	Date	ddmmyy	UTC
12	Magnetic Variation	x.x	degrees
13	East or West (for previous)	x	E or W
14	Mode	x	alphanumeric
15	Checksum	xx	UTC

INVTG: Speed Over Ground, Course Over Ground

14+025:23:59:59.100 \$INVTG,32.69,T,,M,10.6,N,19.6,K,A*1A

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPVTG		
3	Heading	x.xx	degrees
4	T = True (for previous)	x	T
5	Heading	x.xx	degrees
6	M = Magnetic (for previous)	x	M
7	Speed over Ground (knots)	x.x	knots
8	N = knots (for previous)	x	N
9	Speed over Ground (kilometers per hour)	x.x	km/h
10	K = km per hour (for previous)	x	K
11	Mode*	X	A,D,E, or N
12	Checksum	xx	alphanumeric

PSXN,20: Data Quality

10+351:23:59:58.200 \$PSXN,20,1,2,0,0*38

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$PSXN		
3	20		
4	Horizontal position and velocity quality	x	0,1,2
5	Height and vertical velocity quality	x	0,1,2
6	Heading quality	x	0,1,2
7	Roll and pitch quality	x	0,1,2
8	Checksum	xx	alphanumeric

Quality flags: 0 = normal, 1 = reduced performance, 2 = invalid data

PSXN,23: Roll, Pitch, Heading and Heave

10+351:23:59:58.213 \$PSXN,23,0.02,-0.76,330.56,*0B

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$PSXN		
3	23		
4	Roll, port side up is positive	x.xx	degrees
5	Pitch, bow up is positive	x.xx	degrees
6	Heading, True	x.xx	degrees
7	Heave, positive is down	x.xx	m
8	Checksum	xx	alphanumeric

Igar - Garmin GPS***RMC: Recommended Minimum for Navigation***

15+051:21:02:04.741

\$GPRMC,210204.38,A,7712.979182,S,16741.063669,W,9.4,270.82,200215,105.6,E,A*06

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPRMC		
3	Time	hhmmss.sss	UTC
4	Status*	x	A or N
5	Latitude	ddmm.mmmmmm	degrees
6	North or South (for previous)	x	N or S
7	Longitude	ddmm.mmmmmm	degrees
8	East or West (for previous)	x	E or W
9	Speed over Ground, True	x.x	knots
10	Course over Ground True	x.xx	degrees
11	Date	ddmmyy	UTC
12	Magnetic Variation	x.x	degrees
13	East or West (for previous)	x	E or W
14	Mode*	x	alphanumeric
15	Checksum	xx	UTC

GGA: Global Positioning Fix Data

08+034:12:26:06.131 \$GPGGA,122607,6446.4733,S,06403.4455,W,1,11,0.9,-193.4,M,9.7,M,,*5A

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$INGGA		
3	Time	hhmmss.ss	UTC
4	Latitude in degrees with decimal minutes	ddmm.mmmmmm	degrees
5	North or South (for previous)	x	N or S
6	Longitude in degrees with decimal minutes	ddmm.mmmmmm	ddmm.mmmmmm
7	East or West (for previous)	x	E or W
8	GPS quality indicator	x	0 – 6
9	Number of satellites in use (00-99)	xx	00-99
10	Horizontal dilution of precision (HDOP)	x.x	
11	Antenna height	x.xx	meters
12	M = meters (for previous)	X	M
13	Geoidal separation	x.xx	meters
14	M = meters (for previous)	X	M
15	Age of DGPS corrections (null with no DGPS)	x.x	seconds
16	If used, ID of DGPS reference station	Xxxx	0000 - 1023

GLL: (obsolete) Geographic Position

16+077:00:00:00.725 \$GPGLL,6356.6505,S,05716.0002,W,000000,A,A*4F

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPGLL		
3	Latitude	ddmm.mmmmmm	degrees
4	North or South (for previous)	x	N or S
5	Longitude	ddmm.mmmmmm	degrees
6	East or West (for previous)	x	E or W
7	Time of Position (not received)	hhmmss.ss	UTC
8	Status*	x	A or V
9	Mode*	x	alphanumeric
10	Checksum	xx	alphanumeric

Status

A = Data Valid, V = Data not valid

Modes

A = GPS used, D = DGPS used, E = Dead reckoning used, M = Manual input mode, S = Simulator Mode, N = Invalid position / velocity

GPVTG: Track Made Good and Speed over Ground

15+051:16:47:06.625 \$GPVTG,357.84,T,251.99,M,9.5,N,17.7,K,A*15

Field	Data	Format	Unit
1	RVDAS time tag	yy+ddd:hh:mm:ss.sss	UTC
2	\$GPVTG		
3	Heading	x.xx	degrees
4	T = True (for previous)	x	T
5	Heading	x.xx	degrees
6	M = Magnetic (for previous)	x	M
7	Speed over Ground (knots)	x.x	knots
8	N = knots (for previous)	x	N
9	Speed over Ground (kilometers per hour)	x.x	km/h
10	K = km per hour (for previous)	x	K
11	Mode*	X	A,D,E, or N
12	Checksum	xx	alphanumeric

Modes

A = GPS used, D = DGPS used, E = Dead reckoning used, N = Invalid position / velocity

lais – AIS receiver

AIVDM: AIS Data

14+070:00:02:38.575 !AIVDM,1,1,,B,15O5G4000oKPfggK2F2RQj7>0@FU,0*04

Field	Data	Units
1	RVDAS Time Tag	
2	!AIVDM	
3	Total number of sentences needed to transfer the message	(1 – 9)
4	Message Sentence Number	(1 – 9)
5	Sequential identifier to link multiple messages	(0 – 9 or null)
6	AIS Channel	A or B
7	Encapsulated Binary Coded Data ¹	ASCII text
8	Number of fill bits	(0 – 5)
15	*Check sum	hexadecimal

¹Data is encoded as described in ITU-R M.1371

LMG Sensors

Shipboard Sensors

Sensor	Description	Serial #	Cal. Date	Status
Port Anemometer	Gill Ultrasonic Wind Observer II	1246001-WC45	N/A	Collected
Starboard Anemometer	Gill Ultrasonic Wind Observer II	1246002-WC45	N/A	Collected
Barometer	R.M. Young 61201	BP01707	12-Aug-2014	Collected
Humidity/Wet Temp	RM Young 41372LC	6133	14-Aug-2014	Collected
PAR for Mast	Biosph. Inst. QSR-240P	6393	31-Mar-2015	Collected
PIR	Eppley PIR	28903F3	3-Feb-2015	Collected
PSP	Eppley PSP	28933F3	3-Feb-2015	Collected
GUV (Mast)	Biosph. Inst. GUV-2511	25110805127	15-Jun-2015	Collected
Transmissometer	WET Labs C-Star 25 cm deep	CST-407DR	21-Aug-2015	Collected
MicroTSG (Primary)	Sea-Bird 45	243	16-May-2014	Collected
MicroTSG (Secondary)	Sea-Bird 45	390	30-Oct-2014	Collected
Digital Remote Temp	Sea-Bird 38	351	28-Dec-2013	Collected
Fluorometer	WET Labs ECO-FL	FLRTD-380	24-Oct-2014	Collected

Underway Calibration Sheets

Anemometer- Port

WindObserver II™

Product Test Report


Product Tested: WindObserver II

Part Number: 1390-70-B-322

Serial Number: 1246001 - WC45

Test Date: 16/11/2012

Location: Gill Instruments Ltd



GILL ensures that quality is inherent in all aspects of the activities and ensures that compliance with BS EN ISO9001: 2008 is maintained.

This report certifies that the above instrument has been tested in accordance with Gill internal procedures


Results

Test	Limits	Passed
Still Air Test (Zero Wind Speed)	< 0.02m/s	Pass
Wind Tunnel Test (12 m/s nominal)	Pass/Fail	Pass

Generic calibration is traceable to the University of Southampton wind tunnel and instrumentation is maintained in accordance with UKAS.


All tests have been successfully completed

On behalf of Gill Instruments Ltd




Tony Raine
Quality Control

2002-0395 Issue 1



Gill Instruments Ltd
Solihull Park
67 Gosport Street
Lynton
Hampshire
SO41 9SG, UK

T: +44 (0) 1590 613 500
F: +44 (0) 1590 613 535
E: enquiries@gill.co.uk
www.gill.co.uk



Copyright © Gill Instruments 2011

Gill Instruments Ltd
Reg No. 31 04 52 Registered Office: The George Business Centre, Christchurch Road, New Milton, BH23 6DJ

*Anemometer-Starboard***WindObserver II™****Product Test Report****Product Tested: WindObserver II****Part Number: 1390-70-B-322****Serial Number: 1246002 - WC45****Test Date: 15/11/2012****Location: Gill Instruments Ltd**

GILL ensures that quality is inherent in all aspects of the activities and ensures that compliance with BS EN ISO9001: 2008 is maintained.

This report certifies that the above instrument has been tested in accordance with Gill internal procedures

Results

Test	Limits	Passed
Still Air Test (Zero Wind Speed)	< 0.02m/s	Pass
Wind Tunnel Test (12 m/s nominal)	Pass/Fail	Pass

Generic calibration is traceable to the University of Southampton wind tunnel and instrumentation is maintained in accordance with UKAS.

All tests have been successfully completed

On behalf of Gill Instruments Ltd

Tony Raine
Quality Control

2002-0395 Issue 1



Gill Instruments Ltd
Lymington Road
Lymington
Hants PO30 2PP, UK

T: +44 (0) 1590 613 500
F: +44 (0) 1590 613 505
E: info@gill.co.uk

www.gill.co.uk



Copyright © Gill Instruments 2012

Gill Instruments Ltd
Print No: 01246 Wind Observer II Starboard Test Report
Gill Instruments Revision No: 01 (2012)

Barometer

R.M. Young Company
2901 Aero Park Drive
Troy, Michigan 48066 USA



CALIBRATION REPORT
Barometric Pressure

Customer: *Lockheed Martin Corp*

Test Number: 4812-01B

Customer PO: 4900051187

Test Date: 12 August 2014

Sales Order: 4249

<u>Test Sensor:</u>
Model: E1201
Description: Barometric Pressure Sensor
Serial Number: BP01707

Report of calibration comparison of test barometric pressure sensor with National Institute of Standards and Technology traceable standard pressure calibrator at five pressures in the R.M. Young Company controlled pressure facility. Calibration accuracy ± 1.0 hPa.

Reference Pressure (hPa)	Voltage Output (millivolts)	Indicated (1) Pressure (hPa)
800.0	0	800.0
875.0	1261	876.0
950.0	2501	950.1
1025.0	3750	1025.0
1100.0	4997	1089.8

(1) Calculated from voltage output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument:

Druck Pressure Controller Model DPI515

Fluke Multimeter Model 8060A

Serial # NIST Test Reference

51500497 UKAS Lab 0221

4865407 234027

Tested By: 

METEOROLOGICAL INSTRUMENTS
Tel: 248-946-3660 Fax: 248-946-4777 email: sales@youngusa.com Website: youngusa.com
ISO 9001:2008 CERTIFIED

Air Temperature / Relative Humidity

R.M. Young Company
2001 Acorn Park Drive
Livestock City, Michigan 49666 USA

CALIBRATION REPORT Temperature

Customer: *Lockheed Martin Corp*

Test Number: 4814-08T

Customer PO: 4900051188

Test Date: 14 August 2014

See as Order: 4250

Test Sensor:

Model: 41372LC

Serial Number: 7506133

Description: Temperature/Relative Humidity Sensor

Report of calibration comparison of test temperature sensor with National Institute of Standards and Technology traceable standard thermometers at three temperatures in the R.M. Young Company controlled temperature calibration bath facilities. Calibration accuracy: 0.1° Celsius.

Bath Temperature (degrees C)	Current Output (milliamps)	Indicated (1) Temperature (degrees C)
-50.00	4.001	-49.98
-0.01	11.987	0.02
49.94	19.989	49.93

(1) Calculated from current output

All reference equipment used in this calibration procedure have been tested by comparison to traceable standards certified by the National Institute of Standards and Technology.

Reference Instrument:

Brooklyn Thermometer Model 43-FC
Brooklyn Thermometer Model 22332-D5-FC
Brooklyn Thermometer Model 2X430-D7-FC
Keithley Multimeter Model 181

Serial # NIST Test Reference

3006 118 W204690
25071 W204691
77532 W204692
15232 4200640497

Tested By: *R. Thullen*

METEOROLOGICAL INSTRUMENTS
Tel: 231-848-3680 Fax: 231-848-4772 E-mail: info@youngusa.com Website: www.youngusa.com
ISO 9001:2008 CERTIFIED

*PAR for mast***Biospherical Instruments Inc.**

CALIBRATION CERTIFICATE

Calibration Date	3/31/2015
Model Number	QSR240
Serial Number	6393
Operator	TPC
Standard Lamp	V-033(3/3/15)
Probe Excitation Voltage Range:	6 to 18 VDC(+)
Output Polarity:	Positive

Probe Conditions at Calibration (in air):

Calibration Voltage:	6 VDC(-)
Probe Current:	1.3 mA

Probe Output Voltage:

Probe Illuminated	97.9 mV
Probe Dark	0.4 mV
Probe Net Response	97.5 mV
RG780	0.4 mV

Corrected Lamp Output:

Output In Air (same condition as calibration):

9.391E+15	quanta/cm ² sec
155.94603	μE/m ² sec

Calibration Scale Factor:

(To calculate irradiance, divide the net voltage reading in Volts by this value.)

Dry:	1.0379E-17	V/(quanta/cm ² sec)
	6.2504E-04	V/(μE/m ² sec)

Notes:

1. Annual calibration is recommended.
2. Calibration is performed using a Standard of Spectral Irradiance traceable to the National Institute of Standards and Technology (NIST).
3. The collector should be cleaned frequently with alcohol.
4. Calibration was performed with customer cable, when available.

QSR240R 05/24/95

PIR

**THE EPPLEY LABORATORY, INC.**12 Sheffield Avenue, PO Box 419, Newport, Rhode Island USA 02840
Phone: 401.847.1020 Fax: 401.847.1031 Email: info@eppleylab.com**STANDARDIZATION OF
EPPLEY PRECISION INFRARED RADIOMETER
Model PIR**

Serial Number: 28903F3

Resistance: 675 Ω at 23°C

Temperature Compensation Range: -20° to +40°C

This pyrgeometer has been compared against Eppley's Blackbody Calibration System under radiation intensities of approximately 200 watts meter⁻² and an average ambient temperature of 25°C as measured by Standard Omega Temperature Probe, RTD#1.

As a result of a series of comparisons, it has been found to have a sensitivity of:

$$3.57 \times 10^{-6} \text{ volts/watts meter}^{-2}$$

The calculation of this constant is based on the fact that the relationship between radiation intensity and emf is rectilinear to intensities of 700 watts meter⁻². This radiometer is linear to within $\pm 1.0\%$ up to this intensity.

The calibration of this instrument is traceable to the International Practical Temperature Scale (IPTS) through a precision low-temperature blackbody.

Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy. Unless otherwise stated in the remarks section below or on the Sales Order, the results are "AS FOUND / AS LEFT".

Shipped to: LMP4 ISGS(NSF)
Port Hueneme, CA

Date of Test: February 3, 2015

S.O. Number: 64325
Date: February 3, 2015

In Charge of Test:

Reviewed by:

Remarks:

End of Report

**THE EPPLEY LABORATORY, INC.**

12 Sheffield Avenue, PO Box 419, Newport, Rhode Island USA 02840
Phone: 401.847.1020 Fax: 401.847.1031 Email: info@eppleylab.com

Calibration Certificate

Instrument: Precision Spectral Pyranometer, Model PSP, Serial Number 28933F3

Procedure: This pyranometer was compared in Eppley's Integrating Hemisphere according to procedures described in *ISO 9847 Section 5.3.1* and Technical Procedure, TP01 of The Eppley Laboratory, Inc.'s Quality Assurance Manual on Calibrations.

Transfer Standard: Eppley Precision Spectral Pyranometer, Model PSP, Serial Number 21231F3

Results: **Sensitivity:** $S = 8.13 \mu V / W m^{-2}$
Uncertainty: $U_{95} = \pm 0.91\%$ (95% confidence level, k=2)
Resistance: 686 Ω at 23°C


Date of Test: February 3, 2015

Traceability: This calibration is traceable to the World Radiation Reference (WRR) through comparisons with Eppley's AHF standard self calibrating cavity pyrheliometers which participated in the Eleventh International Pyrheliometric Comparisons (IPC XI) at Davos, Switzerland in September-October 2010. Unless otherwise stated in the remarks section below or on the Sales Order, the results of this calibration are "AS FOUND / AS LEFT".

Due Date: Eppley recommends a minimum calibration cycle of five (5) years but encourages annual calibrations for highest measurement accuracy.

Customer: LMP4 ISGS(NSF)
Port Hueneme, CA

Signatures: In Charge of Test: 

Reviewed by: 

Eppley SO: 64325

Date of Certificate: February 3, 2015

Remarks:

End of Report

PSP

GUV



Biospherical Instruments Inc.

GUV-2511 Calibration Certificate										
System Serial Number		25110805127				Date of Calibration		6/15/2015		
Calibration database		25110805127v7.mdb				Date of Certificate		6/15/2015		
DASSN		0111				Standard of Spectral Irradiance		V-033 (3/3/15)		
Microprocessor Tag Number		2				Operator		TC		
Monochromatic Channels	Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	ScaleSmall [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	ScaleMedium [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	ScaleLarge [Volts per $\mu\text{W}/(\text{cm}^2\cdot\text{nm})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
Ed0305	2	305	4.3412E-11	4.4645E-06	1.3124E-03	4.0159E-01	-4.4209E-04	-4.4843E-04	-5.4940E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0313	6	313	1.7792E-10	1.8120E-05	5.3084E-03	1.8643E+00	1.3446E-04	1.4032E-04	1.2464E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0320	8	320	2.5802E-10	2.6271E-05	7.7145E-03	2.5278E+00	-1.8351E-04	-1.8546E-04	6.7677E-05	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0340	10	340	1.9800E-10	2.0210E-05	5.9050E-03	2.1161E+00	1.0116E-04	9.5762E-05	1.2388E-03	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0380	12	380	7.0722E-11	7.2188E-06	2.1141E-03	7.2645E-01	-2.7743E-04	-2.8172E-04	-1.4003E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Ed0395	13	395	2.7486E-10	2.8166E-05	8.2305E-03	2.8018E+00	-2.2586E-04	-2.2546E-04	-4.9964E-04	$\mu\text{W}/(\text{cm}^2\cdot\text{nm})$
Broadband Channels	Address	Wavelength [nm]	Responsivity [Amps per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	ScaleSmall [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	ScaleMedium [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	ScaleLarge [Volts per $\mu\text{E}/(\text{cm}^2\cdot\text{s})$]	OffsetSmall [volts]	OffsetMedium [volts]	OffsetLarge [volts]	Measurement Units
Ed0PAR	18	400-700	1.6871E-05	1.6983E+00	4.9737E+02	1.6394E+05	-1.0804E-04	-1.0693E-04	6.2169E-04	$\mu\text{E}/(\text{cm}^2\cdot\text{sec})$
Auxiliary Channels	Address	Wavelength	Responsivity	ScaleS	ScaleM	ScaleL	OffsetS	OffsetM	OffsetL	Measurement Units
Ed0Temp	22	0	1	0.01	0.01	0.01	0	0	0	$^{\circ}\text{C}$
Ed0Vin	27	0	1	-0.25	-0.25	-0.25	0	0	0	V

© Biospherical Instruments Inc., 5340 Riley Street, San Diego, California 92110 USA. Contact support@biospherical.com for more information.

Calibration Data – Do Not Destroy

page 2 of 2

Transmissometer

PO Box 518
620 Applegate St.
Philomath, OR 97370



(541) 929-5850
Fax (541) 929-5277
www.wetlabs.com

C-Star Calibration

Date	8.21.15	S/N#	CST-407DR	Pathlength	25cm
		Analog output	Digital output		
V_d		0.004 V	0 counts		
V_{air}		4.821 V	15832 counts		
V_{ref}		4.699 V	15433 counts		
Temperature of calibration water				24.3	°C
Ambient temperature during calibration				22.8	°C

Relationship of transmittance (Tr) to beam attenuation coefficient (c), and pathlength (x , in meters): $Tr = e^{-cx}$

To determine beam transmittance: $Tr = (V_{sig} - V_{dark}) / (V_{ref} - V_{dark})$

To determine beam attenuation coefficient: $c = -1/x * \ln(Tr)$

V_d Meter output with the beam blocked. This is the offset.

V_{air} Meter output in air with a clear beam path.

V_{ref} Meter output with clean water in the path.

Temperature of calibration water: temperature of clean water used to obtain V_{ref} .

Ambient temperature: meter temperature in air during the calibration.

V_{sig} Measured signal output of meter.

Revision L

6/9/09

*Thermosalinograph (Temperature) – Primary***Sea-Bird Electronics, Inc.**

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0243
CALIBRATION DATE: 16-May-14SBE 45 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

COEFFICIENTS:


a0 = 1.417246e-005
a1 = 2.749041e-004
a2 = -2.553507e-006
a3 = 1.527836e-007

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	759568.9	1.0000	-0.0000
4.5000	647915.0	4.5000	0.0000
15.0000	410152.8	14.9999	-0.0001
18.5000	354383.2	18.5001	0.0001
24.0000	283362.0	24.0000	-0.0000
29.0000	232648.2	29.0000	0.0000
32.5000	203331.4	32.5000	-0.0000

Temperature ITS-90 = $1/\{a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]\} - 273.15$ (°C)

Residual = instrument temperature - bath temperature

n = instrument output

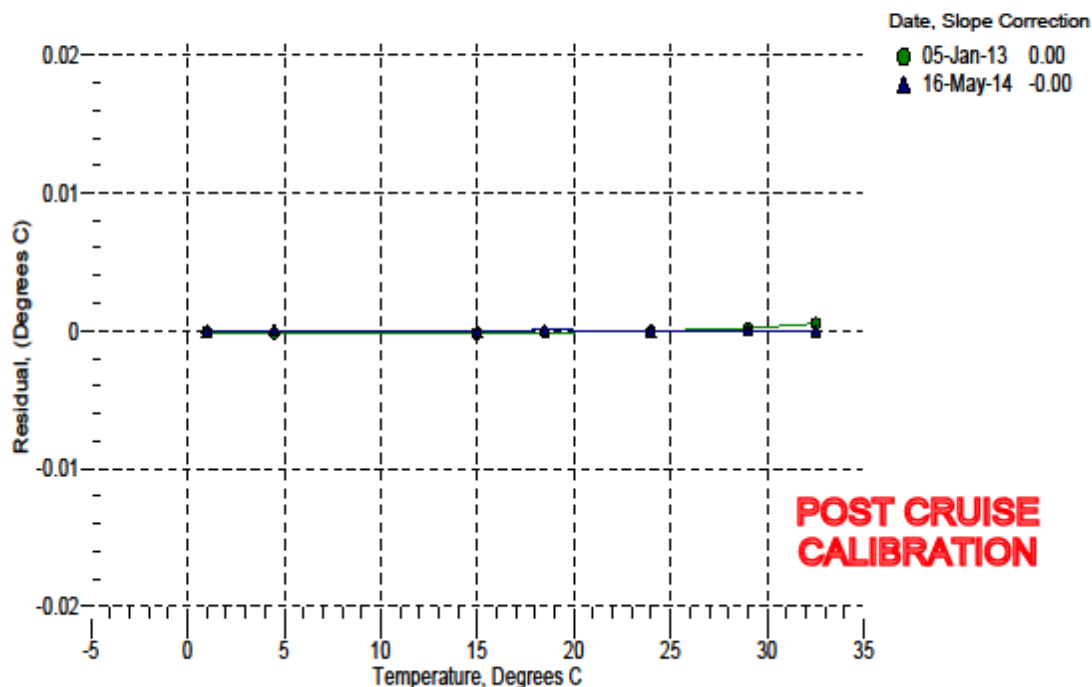

*Thermosalinograph (Conductivity) - Primary***Sea-Bird Electronics, Inc.**

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0243
CALIBRATION DATE: 16-May-14SBE 45 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

COEFFICIENTS:

g = -1.008861e+000
h = 1.574112e-001
i = -3.646901e-004
j = 5.431565e-005CPcor = -9.5700e-008
CTcor = 3.2500e-006
WBOTC = 1.1173e-006


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (Hz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2536.23	0.00000	0.00000
1.0000	34.6704	2.96468	5031.60	2.96467	-0.00001
4.5000	34.6504	3.27061	5221.13	3.27062	0.00001
15.0000	34.6078	4.24873	5784.74	4.24873	-0.00000
18.5000	34.5989	4.59263	5969.99	4.59263	-0.00000
24.0000	34.5892	5.14857	6257.55	5.14856	-0.00000
29.0000	34.5834	5.66845	6514.65	5.66846	0.00001
32.5000	34.5796	6.03937	6691.83	6.03936	-0.00000

$$f = \text{INST FREQ} * \sqrt{1.0 + \text{WBOTC} * t} / 1000.0$$

$$\text{Conductivity} = (g + h * f^2 + i * f^3 + j * f^4) / (1 + \delta * t + \epsilon * p) \text{ Siemens / meter}$$

$$t = \text{temperature} [^{\circ}\text{C}]; p = \text{pressure} [\text{decibars}]; \delta = \text{CTcor}; \epsilon = \text{CPcor};$$

$$\text{Residual} = \text{instrument conductivity} - \text{bath conductivity}$$

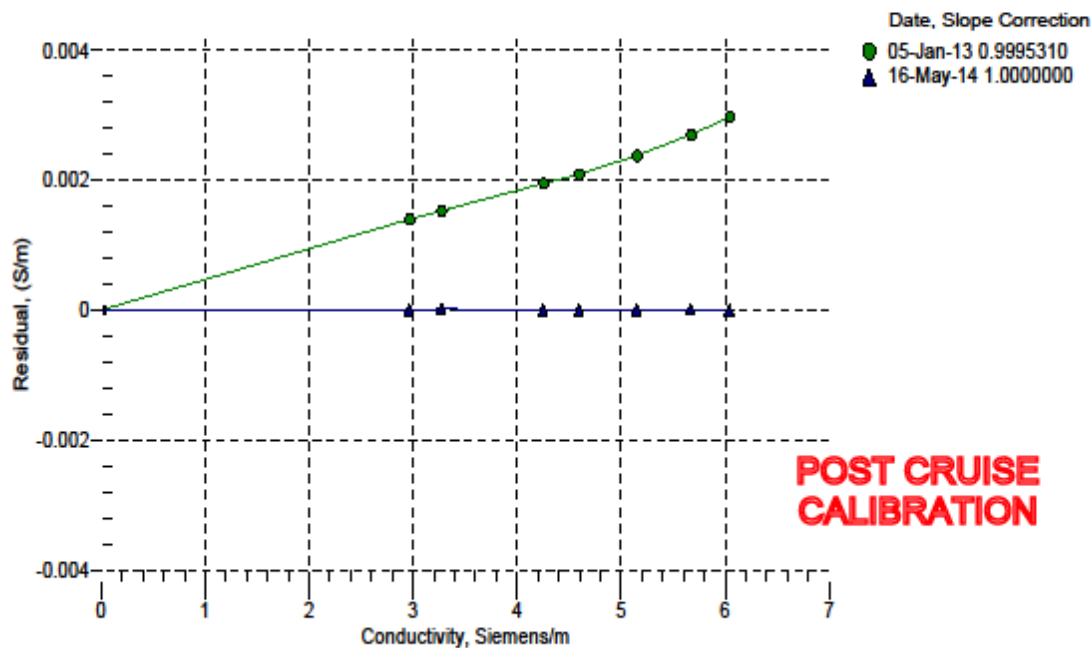

*Thermosalinograph (Temperature) – Secondary***Sea-Bird Electronics, Inc.**

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0390
CALIBRATION DATE: 30-Oct-14SBE 45 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

COEFFICIENTS:


$a_0 = 8.496577\text{e-}006$
 $a_1 = 2.825921\text{e-}004$
 $a_2 = -3.093430\text{e-}006$
 $a_3 = 1.690910\text{e-}007$

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	662306.1	1.0000	0.0000
4.5000	565262.5	4.5000	-0.0000
15.0000	358389.6	15.0000	0.0000
18.5000	309815.7	18.5000	-0.0000
24.0000	247915.6	23.9999	-0.0001
29.0000	203683.3	29.0001	0.0001
32.5000	178100.4	32.5000	-0.0000

$$\text{Temperature ITS-90} = 1/\{a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]\} - 273.15 \text{ (}^\circ\text{C)}$$

Residual = instrument temperature - bath temperature

n = instrument output

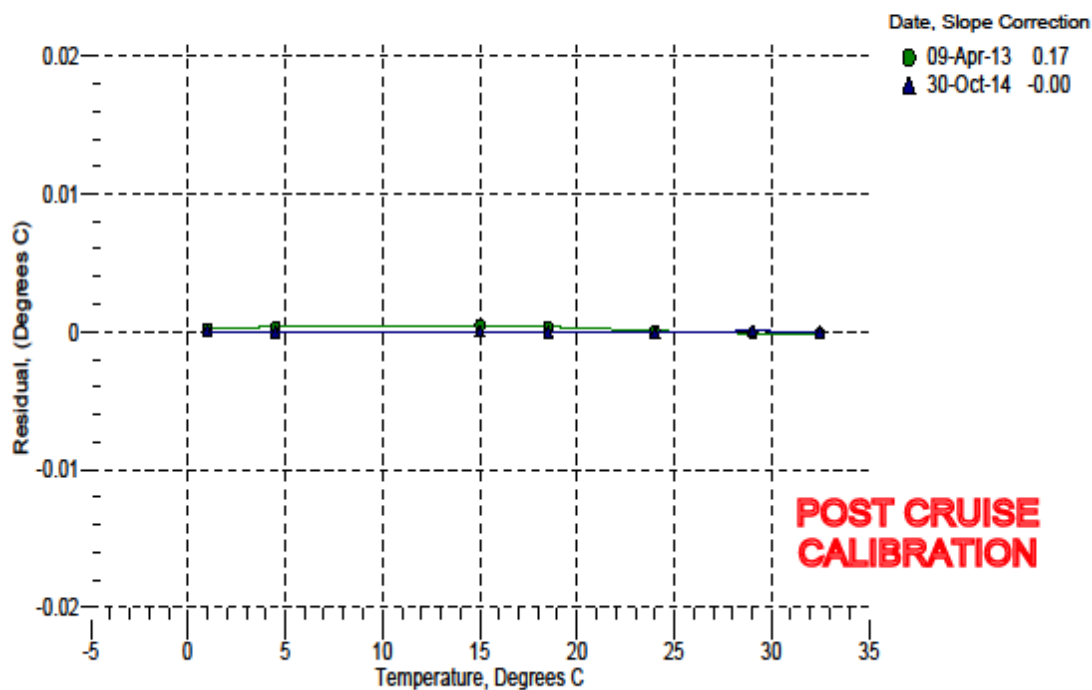

*Thermosalinograph (Conductivity) – Secondary***Sea-Bird Electronics, Inc.**

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0390
CALIBRATION DATE: 30-Oct-14SBE 45 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

COEFFICIENTS:

g = -9.863328e-001
h = 1.453844e-001
i = -4.104173e-004
j = 5.237151e-005CPcor = -9.5700e-008
CTcor = 3.2500e-006
WBOTC = 2.8724e-007


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (Hz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2611.09	0.00000	0.00000
1.0000	34.6932	2.96644	5227.11	2.96644	-0.00000
4.5000	34.6730	3.27253	5425.21	3.27254	0.00001
15.0000	34.6287	4.25103	6014.01	4.25103	-0.00000
18.5000	34.6182	4.59492	6207.39	4.59491	-0.00000
24.0000	34.6058	5.15076	6507.48	5.15076	-0.00000
29.0000	34.5974	5.67049	6775.69	5.67050	0.00001
32.5000	34.5926	6.04138	6960.54	6.04137	-0.00001

$$f = \text{INST FREQ} * \text{sqrt}(1.0 + \text{WBOTC} * t) / 1000.0$$

$$\text{Conductivity} = (g + h * f^2 + i * f^3 + j * f^4) / (1 + \delta * t + \epsilon * p) \text{ Siemens / meter}$$

$$t = \text{temperature} [^{\circ}\text{C}]; p = \text{pressure} [\text{decibars}]; \delta = \text{CTcor}; \epsilon = \text{CPcor};$$

$$\text{Residual} = \text{instrument conductivity} - \text{bath conductivity}$$

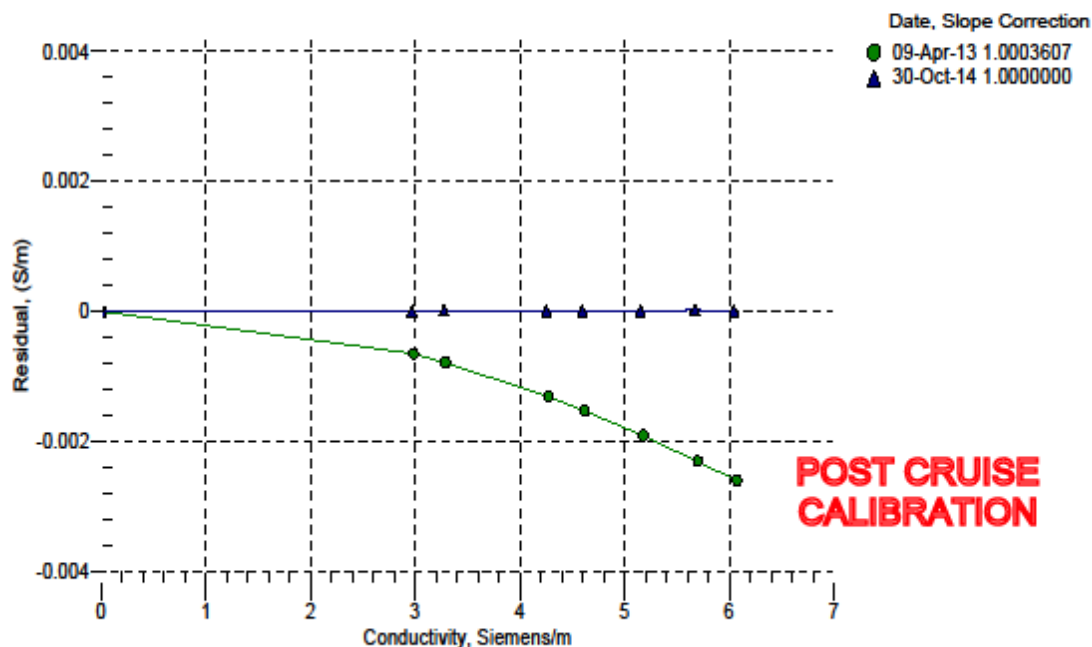

*Digital Remote Temperature***Sea-Bird Electronics, Inc.**

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMRFR: 0351
CALIBRATION DATE: 28-Dec-13SBE 38 TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE


ITS-90 COEFFICIENTS

$a_0 = 6.847307\text{e-}005$
 $a_1 = 2.737587\text{e-}004$
 $a_2 = -2.376425\text{e-}006$
 $a_3 = 1.515438\text{e-}007$

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
-1.50000	674751.5	-1.49996	0.00004
1.00000	601342.4	0.99997	-0.00003
4.50020	513289.0	4.50015	-0.00005
8.00000	439602.0	7.99997	-0.00003
11.50000	377712.0	11.50004	0.00004
14.99990	325560.5	15.00003	0.00013
18.50020	281469.0	18.50008	-0.00012
22.00000	244073.8	22.00011	0.00011
25.50000	212261.3	25.49992	-0.00008
29.00010	185112.4	29.00003	-0.00007
32.50010	161877.4	32.50017	0.00007

$$\text{Temperature ITS-90} = 1/[a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]] - 273.15 \text{ (}^\circ\text{C)}$$

Residual = instrument temperature - bath temperature

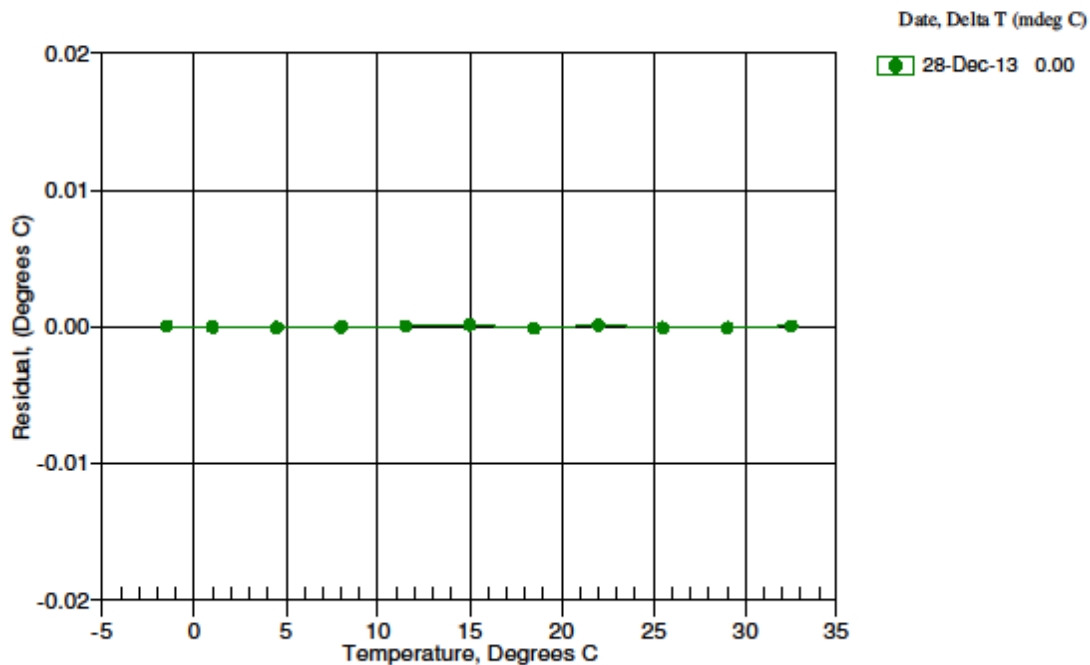

Fluorometer

PO Box 518
620 Applegate St.
Philomath, OR 97370



(541) 929-5650
Fax (541) 929-5277
www.wetlabs.com

ECO Chlorophyll Fluorometer Characterization Sheet

Date: 10/24/2014

S/N: FLRTD-380

Chlorophyll concentration expressed in $\mu\text{g/l}$ can be derived using the equation:

$$\text{CHL } (\mu\text{g/l}) = \text{Scale Factor} * (\text{Output} - \text{Dark Counts})$$

	Analog Range 1	Analog Range 2	Analog Range 4 (default)	Digital
Dark Counts	0.109	0.062	0.040 V	75 counts
Scale Factor (SF)	7	14	28 $\mu\text{g/l/V}$	0.0084 $\mu\text{g/l/count}$
Maximum Output	4.97	4.97	4.97 V	16326 counts
Resolution	0.6	0.6	0.6 mV	0.7 counts

Ambient temperature during characterization

22.3 °C

Analog Range: 1 (most sensitive, 0–4,000 counts), 2 (midrange, 0–8,000 counts), 4 (entire range, 0–16,000 counts).

Dark Counts: Signal output of the meter in clean water with black tape over detector.

SF: Determined using the following equation: $\text{SF} = x \div (\text{output} - \text{dark counts})$, where x is the concentration of the solution used during instrument characterization. SF is used to derive instrument output concentration from the raw signal output of the fluorometer.

Maximum Output: Maximum signal output the fluorometer is capable of.

Resolution: Standard deviation of 1 minute of collected data.

The relationship between fluorescence and chlorophyll-*a* concentrations *in-situ* is highly variable. The scale factor listed on this document was determined using a mono-culture of phytoplankton (*Thalassiosira weissflogii*). The population was assumed to be reasonably healthy and the concentration was determined by using the absorption method. To accurately determine chlorophyll concentration using a fluorometer, you must perform secondary measurements on the populations of interest. This is typically done using extraction-based measurement techniques on discrete samples. For additional information on determining chlorophyll concentration see "Standard Methods for the Examination of Water and Wastewater" part 10200 H, published jointly by the American Public Health Association, American Water Works Association, and the Water Environment Federation.

FLRTD-380

Revision J

3/17/08

Acquisition and Processing Information

Errors and Events

This section lists all significant events and known problems with acquisition during this cruise including instrument failures, data acquisition system failures, and other factors affecting this data set.

On day 094, the order of the last two fields of the MWX string in the met data set was swapped. Both barometers are corrected for sea level. Swap was accomplished because the RMYoung barometer calibration was drifting.

Day Of Year	Time (GMT)	Event	Location
090	02:04	Begin logging	@68W
090	08:00	Garmin GPS stopped producing data	
090	12:20	Power cycled Garmin. Restored data	
091	14:55	ADCP Bottom Tracking Off	Mid Drake
092	14:08	ADCP Bottom Tracking On	Arrive Antarctic shelf
093	10:50	Reset Garmin GPS	
093	11:40	Suspend logging of seawater and sonar	Arrive Palmer Station
093	12:08	Momentary interruption on multiple sensors for equipment reset	
094	19:51	Swapped to using Vaisala barometer vice RMYoung Barometer as primary	
096	21:50	Swapped working tank from 1 to 2 on oxygen system	
100	11:46	Resumed seawater system and sonars	Depart Palmer Station
101	1808	Started new cruise on ADCP to clear tracking errors	
102	2241	ADCP Bottom Tracking On	Arrive Patagonian Shelf
103	2014	End data collection	@68W